

QT-Brightek PLCC Series
PLCC4 RGB LED with Lens

Part No.: QBLP677AD-RGB5

RGB5: White Face, Clear Lens

Product: QBLP677AD-RGB5	Date: November 20, 2022	Page 1 of 10
	Version# 1.2	



Table of Contents:

Introduction 3
Electrical / Optical Characteristic ($T_A=25\text{ }^\circ\text{C}$)..... 4
Absolute Maximum Rating 4
Solder Profile & Footprint..... 7
Packing 8
Ordering Information 9
Revision History 10
Disclaimer 10

Product: QBLP677AD-RGB5	Date: November 20, 2022	Page 2 of 10
	Version# 1.2	

Introduction

Feature:

- Clear lens
- White face
- Package in tape and reel
- Ultra bright PLCC4 RGB LED
- Common Anode
- InGaN technology for IB/IG
- AlInGaP technology for R
- Viewing angle: 30 deg typ.

Description:

This PLCC4 RGB LEDs have a built in lens that provides narrow viewing angle. It is suitable for signage application.

Application:


- Status indication
- Signage
- Signaling

Certification & Compliance:

- TS16949
- ISO9001
- RoHS Compliant



Dimension:

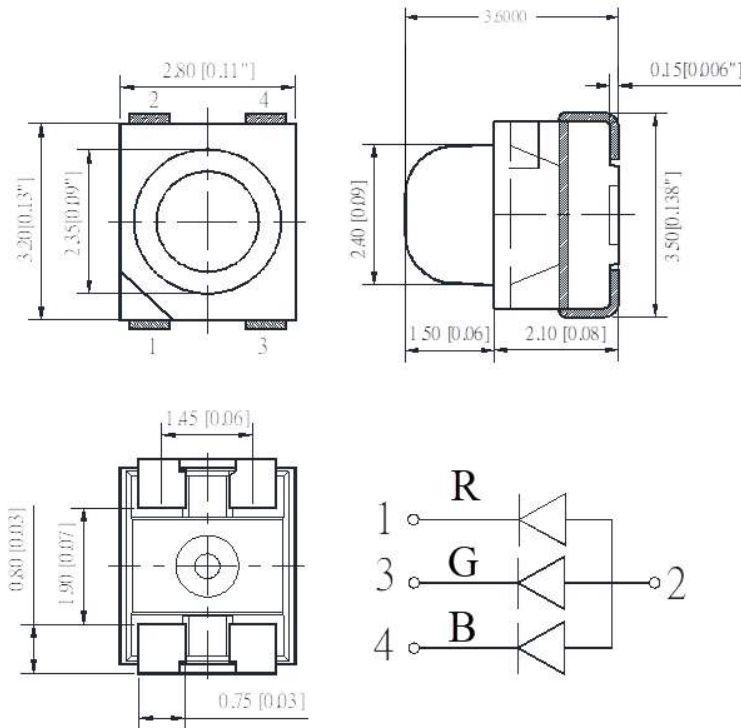

Units: mm / tolerance = +/-0.2mm

Electrical / Optical Characteristic (T_A=25 °C)

Product	Color	I _F (mA)	V _F (V)			λ _D (nm)			I _V (mcd)	
			Min.	Typ.	Max.	Min.	Typ.	Max.	Min.	Typ.
QBLP677AD- RGB5	Red	20	1.7	2.0	2.5	615	622	630	250	550
	True Green	20	2.5	2.8	3.4	520	525	530	2000	4500
	Blue	20	2.8	3.1	3.7	460	465	470	250	500

Absolute Maximum Rating

Material	P _d (mW)	I _F (mA)	I _{FP} (mA)*	V _R (V)	T _{OP} (°C)	T _{ST} (°C)	T _{SO L} (°C)**
AllnGaP (R)	75	30	125	5	-40 to +80	-40 to +85	240
InGaN (IB/IG)	111	30	125	5	-40 to +80	-40 to +85	240

*Duty 1/8 @ 1kHz

**IR Reflow for no more than 10 sec @ 260 °C

Luminous Intensity I_V for Red @ I_F=20mA

Bin	Min.	Max.	Unit
A	250	450	mcd
B	450	650	
C	650	800	

Luminous Intensity I_V for True Green @ I_F=20mA

Bin	Min.	Max.	Unit
D	2000	3300	mcd
E	3300	5000	
F	5000	6800	

Luminous Intensity I_V for Blue @ I_F=20mA

Bin	Min.	Max.	Unit
G	250	400	mcd
H	400	640	
I	640	800	

Dominant Wavelength λ_D for Red @ $I_F=20\text{mA}$

Bin	Min.	Max.	Unit
s	615	620	nm
t	620	625	
u	625	630	





Dominant Wavelength λ_D for True Green @ $I_F=20\text{mA}$

Bin	Min.	Max.	Unit
a	520	525	nm
b	525	530	

Dominant Wavelength λ_D for Blue @ $I_F=20\text{mA}$


Bin	Min.	Max.	Unit
c	460	465	nm
d	465	470	

Characteristic Curves

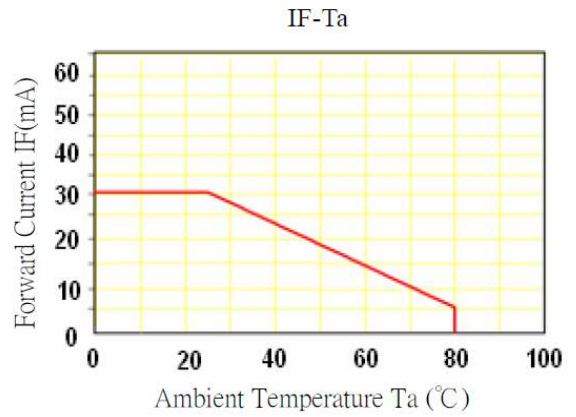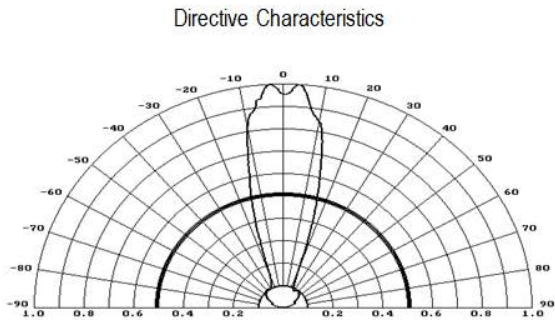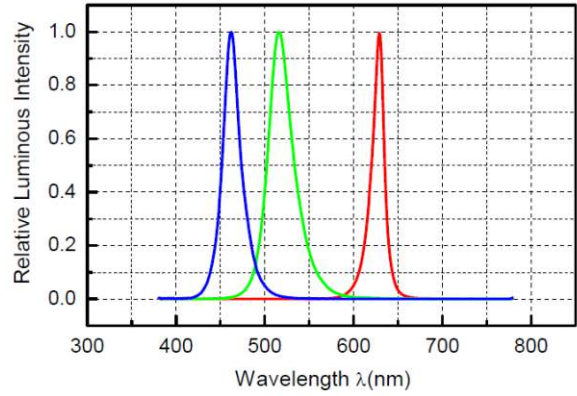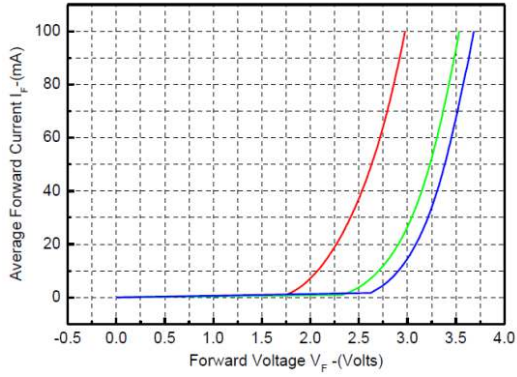


Solder Profile & Footprint

-The recommended reflow soldering profile is as follows (temperatures indicated are as measured on the surface of the LED resin):

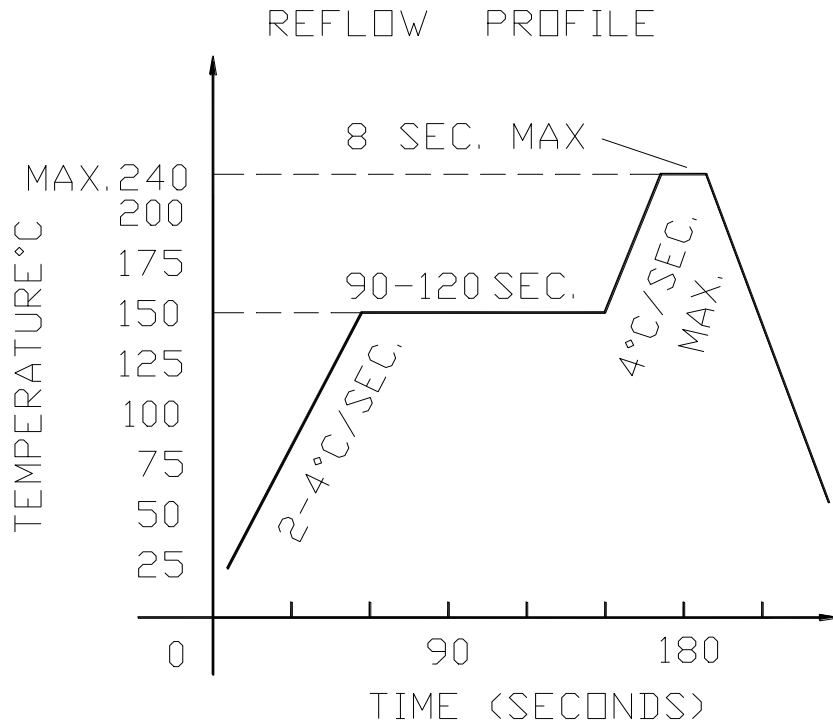


Recommended Pad Layout

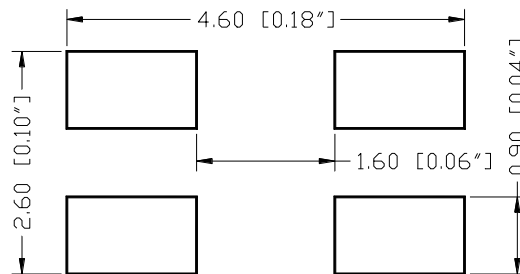

Units: mm


Packing

Reel Dimension:

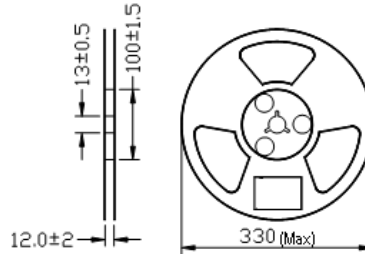


Unit: mm

Tape Dimension:

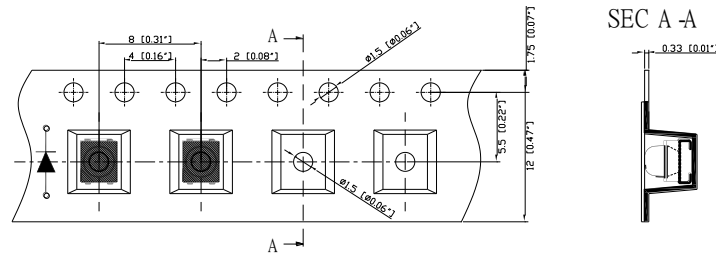


Unit: mm

Arrangement of Tape:

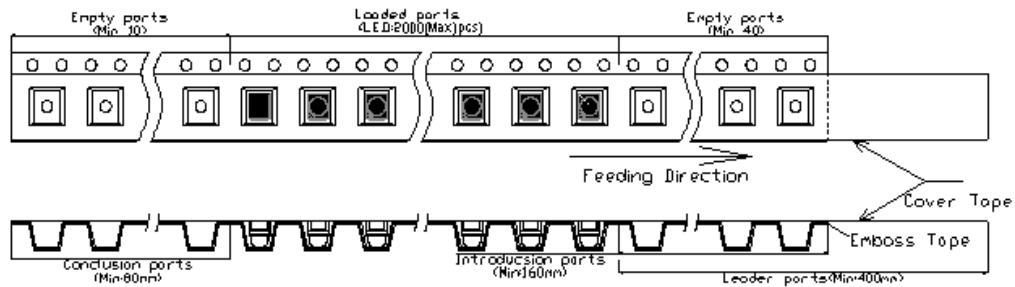

Packaging Specifications:

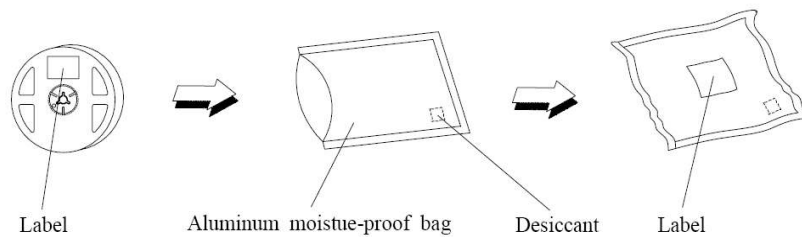

Product: QBLP677AD-RGB5	Date: November 20, 2022	Page 8 of 10
	Version# 1.2	



QBLP677AD-RGB5

PLCC4 RGB LED
with lens

Ordering Information

Part #	Orderable Part #	Spec Range	Quantity per reel
QBLP677AD-RGB5	QBLP677AD-RGB5	Based on page 4 and 5	2,000 units



Revision History

Description:	Revision #	Revision Date
New Release of QBLP677AD-RGB5	V1.0	06/20/2018
Error correction on the drawing dimension	V1.1	11/23/2020
Update brightness and wavelength binning	V1.2	11/20/2022

Disclaimer

QT-BRIGHTTEK reserves the right to make changes without further notice to any products herein to improve reliability, function or design. QT-BRIGHTTEK does not assume any liability arising out of the application or use of any product or circuit described herein; neither does it convey any license under its patent rights, nor the rights of others.

Life Support Policy

QT-BRIGHTTEK's products are not authorized for use as critical components in life support devices or systems without the express written approval of QT-BRIGHTTEK. As used herein:

1. Life support devices or systems are devices or systems which, (a) are intended for surgical implant into the body, or (b) support or sustain life, and (c) whose failure to perform when properly used in accordance with instructions for use provided in the labeling, can be reasonably expected to result in a significant injury of the user.
2. A critical component in any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.

Product: QBLP677AD-RGB5	Date: November 20, 2022	Page 10 of 10
	Version# 1.2	