

# SDM3045X

## Digital Multimeter

DataSheet-2018.12



## Product Overview

SDM3045X is a 4½ digit digital (60000 count) multimeter incorporating a dual-display and is especially well suited for the needs of high-precision, multifunction and automatic measurement.

## User-friendly Design

4.3" TFT-LCD, 480\*272

Support dual display, Chinese and English Menu

Built-in front panel accessible help system

File management (support for U-disc and local storage)

## Main Function

### Basic Measurement Function

- DC Voltage: 600 mV - 1000 V
- DC Current: 600 µA - 10 A
- AC Voltage: True-RMS, 600 mV - 750 V
- AC Current: True-RMS, 60 mA - 10 A
- 2/4-Wire Resistance: 600 Ω - 100 MΩ
- Capacitance: 2 nF - 10000 µF
- Continuity Test: Range is fixed at 2 kΩ
- Diode Test: Adjustable range is 0-4 V.
- Frequency Measurement: 20 Hz - 500 KHz
- Period Measurement: 2 µs - 0.05 s
- Temperature: Support for TC and RTD sensor
- Max, Min, Average, Standard Deviation,  
dBm/dB, Relative Measurement ,Pass/Fail  
Histogram, Trend Chart

### Main Features


- Real 4½ digit (66000 count) readings resolution
- Up to 150 rdgs/s measurement speed
- True-RMS AC Voltage and AC Current measuring
- 1 Gb NAND flash size, Mass storage configuration files and data files
- Built-in cold terminal compensation for thermocouple
- With easy, convenient and flexible PC software: EasyDMM
- Standard interface: USB Device, USB Host, LAN (Optioanal Accessories: USB-GPIB Adapter)
- USB & LAN remote interfaces support common SCPI command set. Compatible with other popular DMMs on the market.

## Special Features


### Histogram




### Trend Chart

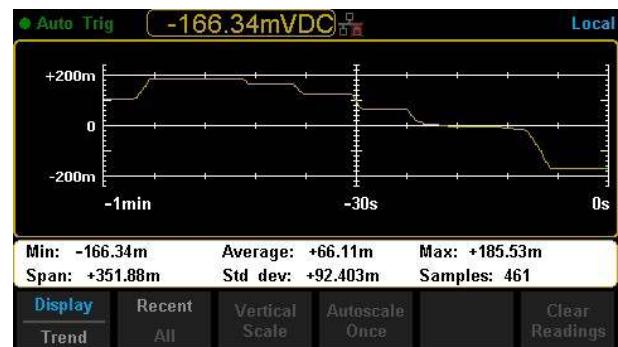


### Bar Chart

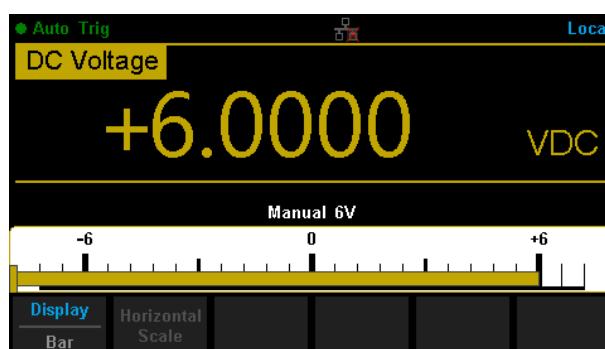


### Statistics

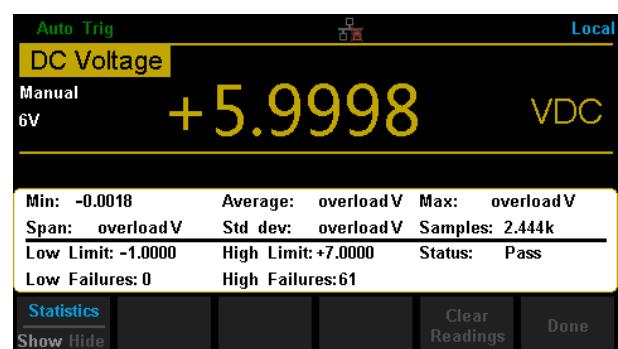


### Dual Display

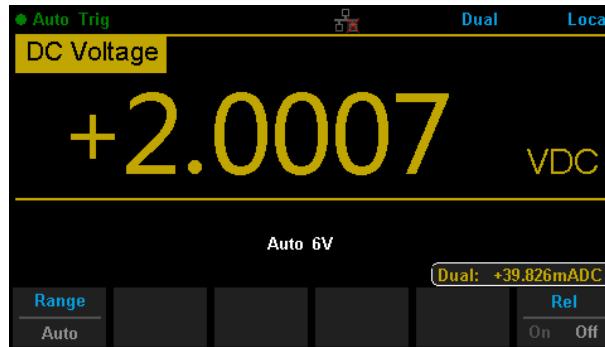

### Hold Measurement

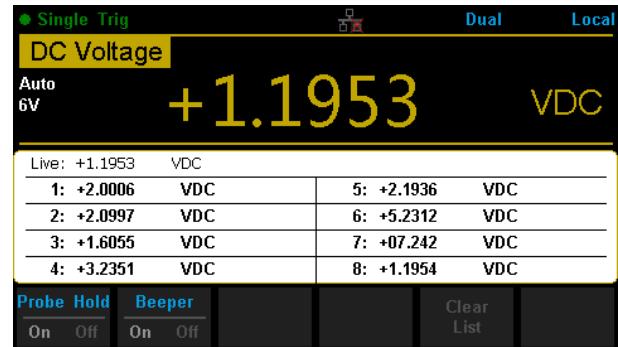

### dBm Hold Measurement

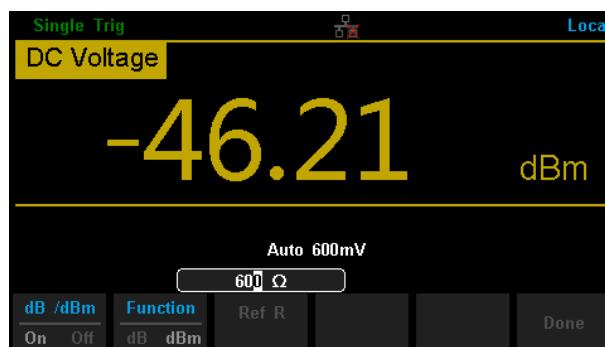

### Interface



## Specifications

### DC Characteristics

Accuracy $\pm$  ( % of Reading + count)<sup>[1]</sup>

Function	Range <sup>[2]</sup>	Test current or Load voltage	Resolution	Accuracy (one year; 23°C ±5°C )
DC Voltage	600 mV		0.01 mV	0.02+ 6
	6 V		0.0001 V	0.02+ 6
	60 V		0.001 V	0.02+ 6
	600 V		0.01 V	0.02+ 6
	1000 V <sup>[4]</sup>		0.1 V	0.02+ 6
DC Current	600 µA	< 33 mV	0.01 µA	0.05+ 3
	6 mA	< 330 mV	0.0001 mA	0.05+ 3
	60 mA	< 0.05 V	0.001 mA	0.05+ 3
	600 mA	< 0.5 V	0.01 mA	0.12+ 6
	6 A	< 0.33 V	0.0001 A	0.20+ 5
	10 A <sup>[5]</sup>	< 0.6 V	0.001 A	0.25+ 4
Resistance <sup>[3]</sup>	600 Ω	1 mA	0.01 Ω	0.08+ 6
	6 KΩ	1 00 µA	0.0001 KΩ	0.04+ 6
	60 KΩ	10 µA	0.001 KΩ	0.04+ 6
	600 KΩ	1 µA	0.01 KΩ	0.08+ 6
	6 MΩ	200 nA	0.0001 MΩ	0.12+ 3
	60 MΩ	200 nA    10 MΩ	0.001 MΩ	0.85+ 3
	100 MΩ	200 nA    10 MΩ	0.01 MΩ	1.75+ 3
Diode Test <sup>[6]</sup>	0-2 V	1 mA	0.0001 V	0.05+ 3
	2-4 V	1 mA	0.0001 V	0.35+ 3
Continuity Test	2000 Ω	1 mA	0.1 Ω	0.05+ 3

### Remarks:

- [1] Specifications are for 0.5 Hour warm-up, "Slow" measurement rate and calibration temperature 18°C - 28°C .
- [2] 10% over range on all ranges except for DCV 1000 V, ACV 750 V, DCI 10 A and ACI 10 A.
- [3] Specifications are for 4-wire measure or 2-wire measure under "REF" operation. ±0.2 Ω of extra errors will be generated if perform 2-wire measure without "REF" operation.
- [4] Plus 0.02 mV of error per 1 V after the first ±500 VDC.
- [5] 30 seconds OFF after 30 seconds ON is recommend for the continuous current that higher than DC 7 A or AC RMS 7 A.
- [6] Accuracy specifications are only for voltage measuring at input terminal. The typical value of current under measure is 1 mA. Voltage drop at diode junction may vary with current supply. Adjustable voltage range : 0- 4 V.



## AC Characteristics

Accuracy $\pm$  ( % of Reading + count)<sup>[1]</sup>

Function	Range <sup>[2]</sup>	Frequency Range	Resolution	Accuracy (one year; 23°C ±5°C )
True-RMS AC Voltage <sup>[3]</sup>	600 mV	20 Hz – 45 Hz	0.01 mV	2.0 + 20
		45 Hz – 100 Hz	0.01 mV	0.6 +10
		100 Hz – 20 KHz	0.01 mV	0.3 + 20
		20 KHz – 50 KHz	0.01 mV	2.0 + 40
		50 KHz –100 KHz	0.01 mV	3.0 + 10
	6 V	20 Hz – 45 Hz	0.0001 V	2.0 + 20
		45 Hz – 100 Hz	0.0001 V	0.6 + 10
		100 Hz – 20 KHz	0.0001 V	0.8 + 20
		20 KHz – 50 KHz	0.0001 V	2.0 + 40
		50 KHz –100 KHz	0.0001 V	3.0 + 40
	60 V	20 Hz – 45 Hz	0.001 V	2.0 + 20
		45 Hz – 100 Hz	0.001 V	0.6 + 10
		100 Hz – 20 KHz	0.001 V	0.8 + 20
		20 KHz – 50 KHz	0.001 V	2.0 + 40
		50 KHz –100 KHz	0.001 V	3.0 + 40
	600 V	20 Hz – 45 Hz	0.01 V	2.0 + 20
		45 Hz – 100 Hz	0.01 V	0.6 + 10
		100 Hz – 20 KHz	0.01 V	0.8 + 20
		20 KHz – 50 KHz	0.01 V	2.0 + 40
		50 KHz –100 KHz	0.01 V	3.0 + 40
	750 V	20 Hz – 45 Hz	0.01 V	2.0 + 20
		45 Hz – 100 Hz <sup>[4]</sup>	0.01 V	0.6 + 10
		100 Hz – 20 KHz	0.01 V	0.8 + 20
		20 KHz – 50 KHz	0.01 V	2.0 + 40
		50 KHz –100 KHz	0.01 V	3.0 + 40
True-RMS AC Current <sup>[5]</sup>	60 mA	20 Hz – 45 Hz	0.001 mA	2.0 + 20
		45 Hz – 2 KHz	0.001 mA	0.5 + 20
		2 KHz – 10 KHz	0.001 mA	2.5 + 30
	600 mA	20 Hz – 45 Hz	0.01 mA	2.0 + 20
		45 Hz – 2 KHz	0.01 mA	0.5 + 20
		2 KHz – 10 KHz	0.01 mA	2.5 + 30
	6 A	20 Hz – 45 Hz	0.0001 A	2.0 + 20
		45 Hz – 2 KHz	0.0001 A	0.5 + 20
		2 KHz – 10 KHz	0.0001 A	2.5 + 20
	10 A <sup>[6]</sup>	20 Hz – 45 Hz	0.001 A	1.5 + 45
		45 Hz – 2 KHz	0.001 A	0.5 + 35
		2 KHz – 10 KHz	0.001 A	2.5 + 25

Additional wave crest factor error ( not Sine )<sup>[7]</sup>

Wave crest coefficient	Error (% Range)
1-2	0.05
2-3	0.3

## Remarks:

[1] Specifications are for 0.5 Hour warm-up, "Slow" measurement rate and calibration temperature 18°C - 28°C .

[2] 10% over range on all ranges except for DCV 1000 V, ACV 750 V, DCI 10 A and ACI 10 A.

[3] Specifications are for amplitude of sine wave input &gt; 5% of range. For inputs from 1% to 5% of range and &lt;50 kHz, add 0.1% of range extra error. For 50 kHz to 100 kHz, add 0.1% of range extra error.

[4] Plus 0.025 V of error per 1 V after the first ±400 VAC.

[5] Specifications are for sine wave input &gt; 5% of range. 0.1% errors will be added when the range of input sine wave is 1% to 5%.

[6] 30 seconds OFF after 30 seconds ON is recommend for the continuous current that higher than DC 7 A or AC RMS 7 A.

[7] For inputs Frequency Range &lt; 100 Hz

## Frequency and Period Characteristic

Accuracy± (% of Reading + count)<sup>[1]</sup>

Function	Range	Frequency Range	Resolution	Accuracy (one year; 23°C ±5°C )
Frequency /Period	600 mV to 750 V <sup>[2]</sup>	20 Hz – 2 KHz		0.01+3
		2 KHz – 20 KHz		0.01+2
		20 KHz – 200 KHz		0.01+2
		200 KHz –500 KHz		0.01+2

## Remarks:

[1] Specifications are for 0.5 Hour warm-up.

[2] Except for special marks, the AC input voltage is 5% to 110% of range when &lt;100 kHz and 10% to 110% of range when &gt;100 kHz. 750 V range is limited to 750 Vrms. The accuracy is 10 times % of Reading when the measurement range of AC voltage is in 600 mV range.

## Capacitance Characteristic

Accuracy± (% of Reading + count)<sup>[1]</sup>

Function	Range <sup>[2]</sup>	Max Testing Current	Resolution	Accuracy (one year; 23°C ±5°C )
Capacitance	2 nF	10 µA	0.001 nF	3+10
	20 nF	10 µA	0.01 nF	1+10
	200 nF	100 µA	0.1 nF	1+9
	2 µF	100 µA	0.001 µF	1+10
	20 µF	1 mA	0.01 µF	1+10
	200 µF	1 mA	0.1 µF	1+9
	10000 µF	1 mA	1 µF	2+50

## Remarks:

[1] Specifications are for 0.5 Hour warm-up and "REF" operation. Using of non-film capacitor may generate additional errors.

[2] Specifications are for from 1% to 110% on 2 nF range and ranges from 10% to 110% on other ranges.

## Temperature Characteristic

Accuracy± (% of Reading)<sup>[1]</sup>

Function	Probe Type	Probe Model	Working Temperature Range	Accuracy (one year; 23°C ±5°C )	Temperature coefficient 0°C - 18°C 28°C - 50°C
Temperature	RTD <sup>[2]</sup>	a=0.00385	-200°C - 660°C	0.16°C	0.09°C
		B	0°C - 1820°C	0.76°C	0.14°C
		E	-270°C - 1000°C	0.5°C	0.02°C
		J	-210°C - 1200°C	0.5°C	0.02°C
		K	-270°C - 1370°C	0.5°C	0.03°C
	TC <sup>[3]</sup>	N	-270°C - 1300°C	0.5°C	0.04°C
		R	-50°C - 1760°C	0.5°C	0.09°C
		S	-50°C - 1760°C	0.6°C	0.11°C
		T	-270°C - 400°C	0.5°C	0.03°C

## Remarks:

[1] Specifications are for 0.5 Hour warm-up, not include probe error.

[2] Specifications are for 4-wire measure or 2-wire measure under "REF" operation.

[3] Built-in cold terminal compensation for thermocouple, accuracy is ±2°C .

## Measuring Method and other Characteristics

<b>DC Voltage</b>		
Input Resistance	600 mV      10 MΩ or 10 GΩ selectable 6 V, 60 V, 600 V and 1000 V Range      10 MΩ ± 2%	
Input Bias Current	<90 pA, 25°C	
Input Protection	1000 V on all ranges	
CMRR	120 dB (For the 1 KΩ unbalanced resistance in LO lead, max ±500 VDC)	
NMRR	60 dB at "slow" measurement rate	
<b>Resistance</b>		
Testing Method	4-wire resistance or 2-wire resistance selectable	
Input Protection	1000 V on all ranges	
<b>DC Current</b>		
Shunt Resistor	600 μA sampling voltage < 33 mV 6 mA sampling voltage < 0.33 V 1Ω for 60 mA, 600 mA 1 Ω 0.01 Ω for 6 A, 10 A	
Input Protection	Rear panel : accessible 10 A, 250 V fast-melt fuse Internal : 12 A, 250 V slow-melt fuse	
<b>Continuity/Diode Test</b>		
Measurement Method	1 mA ±5% constant-current source or open-circuit voltage	
Beeper	yes	
Continuity Threshold	Adjustable	
Input Protection	1000 V	
<b>True-RMS AC Voltage</b>		
Measurement Method	AC Coupled true RMS measure – up to 1000 V DC bias are permitted on every range.	
Wave Crest Factor	≤3 at full scale	
Input Impedance	1 MΩ ± 2% in parallel with <100 pF on all ranges	
AC Filter Bandwidth	20 Hz - 100 KHz	
CMRR	60 dB (For the 1 KΩ imbalance resistance among Lo lead and <60 Hz, Max ±500 VDC)	
<b>True-RMS AC Current</b>		
Measurement Method	DC Coupled to the fuse and shunt; AC Coupled the True-RMS measurement (measures the AC components only)	
Wave Crest Factor	≤3 at full scale	
Max Input	<10 A (include DC component)	
Shunt Resistor	1 Ω for 60 mA, 600 mA 1 Ω; 0.01 Ω for 6 A, 10 A	
Input Protection	Rear panel : accessible 10 A, 250 V fast-melt fuse Internal : 12 A, 250 V slow-melt fuse	
<b>Frequency/Period</b>		
Measurement Method	Reciprocal-counting technique, AC Coupled input, AC voltage or AC current measurement function	
Measure Attentions	errors are leaded into all frequency counters when measuring low voltage or low frequency signal.	
<b>Capacitance Measuring</b>		
Measurement Method	Measure the rate of change of voltage generated during the current flowing the capacitance	
Connection Type	2-wire	
Input Protection	1000 V on all ranges	
<b>Temperature Measuring</b>		
Measurement Method	Support for TC and RTD types of sensor	
<b>Trigger and Memory</b>		
Samples/Trigger	1 - 10000	
Trigger Delay	6 ms - 10000 ms optional	
External Trigger Input	Input Level	TTL compatible (High level when left input terminal is hanging in the air)
	Trigger Condition	Rising and Falling selectable
	Input Impedance	≥20 KΩ/400 pF ,DC-coupled
VMC	Min Pulse	500 us
	Level	TTL compatible
	Output Polarity	Positive and negative optional
	Output Impedance	200 Ω, typical

<b>History Records</b>	
Volatile Memory	10 K reading of history records
Nonvolatile Memory	1 Gb Nand Flash, Mass storage configuration files and data files, Support U-disk external storage
<b>Math Functions</b>	
Min/Max/Average, dBm, dB, Pass/Fail, Relative, Standard deviation, Hold, histogram, Trend chart, Bar chart	

## General Specifications

<b>Power Supply</b>	
AC 100 V - 120 V	45 Hz - 66 Hz
AC 200 V - 240 V	45 Hz - 66 Hz
Consumption	20VA max
<b>Mechanism</b>	
Dimension	293.75 mm×260.27 mm×107.21 mm
Weight	3.76 Kg
<b>Other Characteristics</b>	
Display Screen	4.3" TFT-LCD with resolution 480*272
Operation Environment	Full accuracy from 0°C to 50°C , 80% RH and 40°C , non condensing Storage Temperature: -20°C -70°C Shock and Vibration: conforming to MIL-T-28800E, , 5 level (only for sine) Height above sea level: up to 3000 meters
electromagnetic compatibility	Conforming to EMC (2004/108/EC) and EN 61326-1:2013
Safety	Conforming to EN61010-1:2010 and low voltage instructions (2006/95/EC)
Remote Interface	10/100 Mbit LAN, USB2.0 Full Speed Device and Host
Programmer Language	Standard SCPI, compatible with commands of main stream multimeters
Warm Up Time	30 minutes

## Purchase Information

<b>Standard Accessories</b>	
Power Cord	-1
USB Cable	-1
Quick Start	-1
warranty Card	-1
EasyDMM <sup>[1]</sup>	software system
Test Leads and Alligator Clips	-2
<b>Optional Accessories</b>	
USB-GPIB adapter	USB-GPIB

[1] The latest version of EasyDMM can be downloaded for free from the SDM3000 series of digital multimeter. Please see our web site at [www.siglent.com](http://www.siglent.com) for more information

# SDM3045X

## Digital Multimeter

### About SIGLENT

SIGLENT is an international high-tech company, concentrating on R&D, sales, production and services of electronic test & measurement instruments.

SIGLENT first began developing digital oscilloscopes independently in 2002. After more than a decade of continuous development, SIGLENT has extended its product line to include digital oscilloscopes, function/arbitrary waveform generators, digital multimeters, DC power supplies, spectrum analyzers, isolated handheld oscilloscopes and other general purpose test instrumentation. Since its first oscilloscope, the ADS7000 series, was launched in 2005, SIGLENT has become the fastest growing manufacturer of digital oscilloscopes. We firmly believe that today SIGLENT is the best value in electronic test & measurement.

#### **Headquarter:**

SIGLENT TECHNOLOGIES CO., LTD.  
Add: Bldg No.4 & No.5, Antongda Industrial Zone, 3rd Liuxian Road, Bao'an District, Shenzhen, 518101, China.  
Tel: + 86 755 3661 5186  
Fax: + 86 755 3359 1582  
Email: sales@siglent.com;  
Website: <http://www.siglent.com/ens/>

#### **USA:**

SIGLENT Technologies America, Inc  
6557 Cochran Rd Solon, Ohio 44139  
Tel: 440-398-5800  
Toll Free: 877-515-5551  
Fax: 440-399-1211  
Email: info@siglent.com  
Website: [www.siglentamerica.com](http://www.siglentamerica.com)

#### **Europe:**

SIGLENT TECHNOLOGIES EUROPE GmbH  
ADD: Liebigstrasse 2-20, Gebaeude 14,  
22113 Hamburg Germany  
Tel: +49(0)-819-95946  
Fax: +49(0)-819-95947  
Email: info-eu@siglent.com  
Website: [www.siglenteu.com](http://www.siglenteu.com)

**Follow us on**  
**Facebook: SiglentTech**

