

PGT[®]120.COM Data Terminal 2 (Part No.: 7100.PGT120.COM.DT)


The "Data Terminal 2", is a modular system for recording and processing Personnel Grounding Tester's test data. A basic system consists of: PGT120.COM (1) and Data Terminal (2). Test data can be stored for one month inside the device. The data can be retrieved by a web browser from any computer when connected to a network.

Test data can be imported to Time Attendance or Access Control systems via network interface.

Remote PC functions when connected to network:

- List of measurement data with coloured marking of failed tests
- Printed test results list
- WEB-interface for easy configuration
- German and English support

Overview

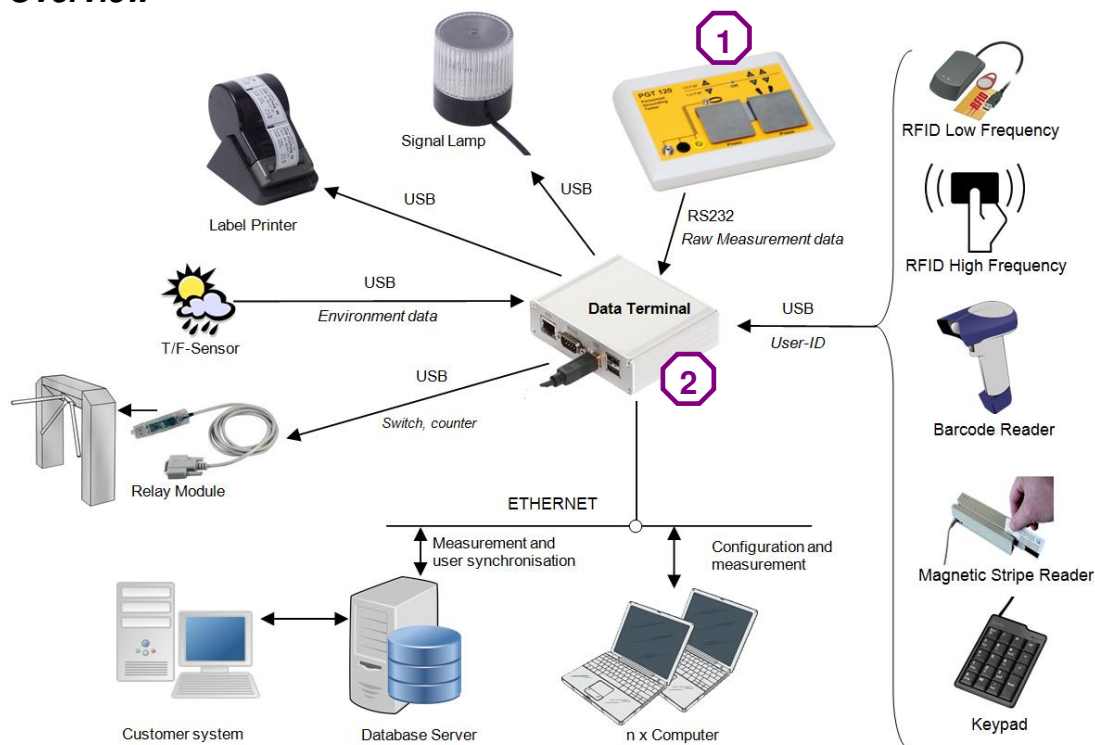

Technical Information

Page 2 of 2

Part No.: 7100.PGT120.COM.DT




Certified by DQS
ISO 9001:2008



◆ Untere Gießwiesen 21 ◆ 78247 Hilzingen ◆ Tel.: +49-7731-86880 ◆ Fax: +49-7731-868830

Interface Connection Example

Two USB ports are available on the Data Terminal. For multiple extensions use a USB-HUB as distributor.

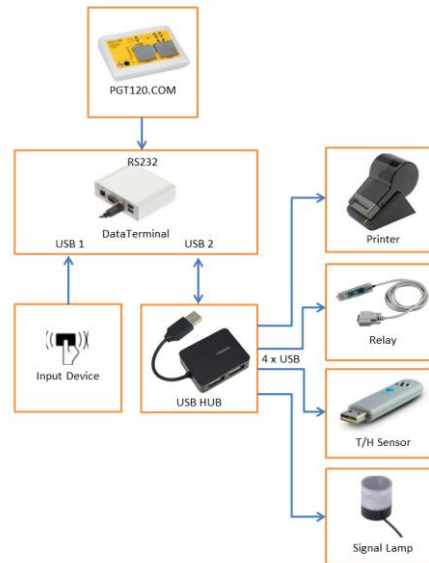

Measurement

Date	Time	Shoe left	Shoe right	Wrist strap	Result	ID	Temp.	RH
2011-02-04	13:37	97.1 MΩ	20.2 MΩ		UserID missing		26.0°C	31.0%
2011-02-04	13:37	58.3 MΩ	21.1 MΩ		UserID missing		26.0°C	31.0%
2011-02-04	13:35			2.6 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.5 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.5 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	21.4 MΩ	27.7 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	23.1 MΩ	27.4 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	25.3 MΩ	27.3 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35	24.4 MΩ	26.1 MΩ		OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			3.3 MΩ	OK	15E8716D	26.0°C	30.5%
2011-02-04	13:35			2.9 MΩ	UserID missing		26.1°C	30.5%
2011-02-04	13:34			2.8 MΩ	OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	23.8 MΩ	25.6 MΩ		OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	23.8 MΩ	26.4 MΩ		OK	15E8716D	26.1°C	30.5%
2011-02-04	13:34	25.9 MΩ	28.3 MΩ		UserID missing		26.1°C	30.5%
2011-02-04	13:24	21.6 MΩ	19.3 MΩ		OK	15E8716D	25.9°C	30.5%
2011-02-04	13:24	23.6 MΩ	20.4 MΩ		UserID missing		25.9°C	30.5%
2011-02-04	11:51	23.4 MΩ	23.3 MΩ		OK	A58FF340	25.4°C	30.5%
2011-02-04	11:51			2.4 MΩ	OK	A58FF340	25.4°C	30.5%
2011-02-04	11:51	23.7 MΩ	25.8 MΩ	2.2 MΩ	OK	A58FF340	25.4°C	30.5%
2011-02-04	11:50	25.7 MΩ	28.5 MΩ		OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50	26.3 MΩ	27.6 MΩ		OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50				Button released too early	15E8716D	25.4°C	30.5%
2011-02-04	11:50			2.3 MΩ	OK	15E8716D	25.4°C	30.5%
2011-02-04	11:50	25.9 MΩ	26.5 MΩ		OK	15E8716D	25.4°C	30.5%

Supplied with:

- Data Terminal
- Power supply
- User's manual (German / English)

PGT120.COM must be ordered separately
Part.-No. 7100.PGT120.COM



▶ 1 year limited warranty

We believe all the information in these pages including technical data to be reliable. However we make no warranties expressed or implied and assume no liability regarding any use of this information.

V0216