

P/N: 71201-0101**Copyright**

© 2023, FLIR Systems, Inc.

All rights reserved worldwide. Names and marks appearing herein are either registered trademarks or trademarks of FLIR Systems and/or its subsidiaries. All other trademarks, trade names or company names referenced herein are used for identification only and are the property of their respective owners.

Document identity

Publ. No.: 71201-0101

Commit: 81601

Language:

Modified: 2021-11-30

Formatted: 2023-02-16

Website

<http://www.flir.com>

Customer support

<http://support.flir.com>

Disclaimer

Specifications subject to change without further notice. Camera models and accessories subject to regional market considerations. License procedures may apply. Products described herein may be subject to US Export Regulations. Please refer to exportquestions@flir.com with any questions.

**General description**

The FLIR AX8 camera/sensor provides an affordable and accurate temperature measurement solution for anyone who needs to solve problems that need built in "smartness" such as analysis, alarm functionality, and autonomous communication using standard protocols. The FLIR AX8 also has all the necessary features and functions to build distributed single- or multi-camera solutions utilizing standard Ethernet hardware and software protocols.

The FLIR AX8 also has built-in support to connect to industrial control equipment such as PLCs, and allows the sharing of analysis and alarm results and simple control using the Ethernet/IP and Modbus TCP field bus protocols.

Key features:

- Support for the EthernetIP field bus protocol (analyze, alarm, and simple camera control).
- Support for the Modbus TCP field bus protocol (analyze, alarm, and simple camera control).
- Built-in analysis functionality.
- Alarm functionality, as a function of analysis and more.
- Built-in web server for control and set up.
- MJPEG, MPEG-4, or H.264 image streaming.
- PoE (Power over Ethernet).
- General-purpose output.
- 100 Mbps Ethernet (100 m cable).
- On alarm: file sending (FTP) or e-mail (SMTP) of analysis results or images.

Typical applications:

- Electrical and mechanical condition-monitoring applications where temperature or temperature trends can be an indication of a potential risk of failure.
- Simple process control applications.

Imaging and optical data

| | |
|--------------------------|-----------------------------------|
| IR resolution | 80 × 60 pixels |
| Thermal sensitivity/NETD | < 0.10°C @ +30°C (+86°F) / 100 mK |
| Field of view (FOV) | 48° × 37° |
| Depth of field | 0.1 m (0.33 ft.), infinity |
| Focal length | 1.54 mm (0.061 in.) |



FLIR AX8 9 Hz

P/N: 71201-0101

© 2023, FLIR Systems, Inc.
#71201-0101; r. 81601;

| Imaging and optical data | |
|---|--|
| Spatial resolution (IFOV) | 11.1 mrad |
| F-number | 1.1 |
| Image frequency | 9 Hz |
| Focus | Fixed |
| Detector data | |
| Detector type | Focal plane array (FPA), uncooled microbolometer |
| Spectral range | 7.5–13 µm |
| Detector pitch | 17 µm |
| Detector time constant | Typical 12 ms |
| Visual camera | |
| Built-in digital camera | 640 × 480 |
| Digital camera, FOV | Adapts to the IR lens |
| Sensitivity | Minimum 10 lux without illuminator |
| Measurement | |
| Object temperature range | -10 to +150°C (14 to +302°F) |
| Accuracy | ±2°C (±3.6°F) or ±2% of reading (+10 to +100°C @ +10 to +35°C ambient) |
| Measurement analysis | |
| Spotmeter | 6 |
| Area | 6 boxes with max./min./average |
| Automatic hot/cold detection | Max./min. temperature value and position shown within box |
| Measurement presets | Yes |
| Atmospheric transmission correction | Automatic, based on inputs for distance, atmospheric temperature and relative humidity |
| Optics transmission correction | Automatic, based on signals from internal sensors |
| Emissivity correction | Variable from 0.01 to 1.0 |
| Reflected apparent temperature correction | Automatic, based on input of reflected temperature |
| External optics/windows correction | Automatic, based on input of optics/window transmission and temperature |
| Measurement corrections | Global object parameters |
| Alarm | |
| Alarm functions | Automatic alarms on any selected measurement function. A maximum of 5 alarms can be set. |
| Alarm output | Digital out, store image, file sending (FTP), email (SMTP), notification |



FLIR AX8 9 Hz

P/N: 71201-0101

© 2023, FLIR Systems, Inc.
#71201-0101; r. 81601;

| Set-up | |
|--------------------------------------|--|
| Color palettes | <ul style="list-style-type: none">• Arctic• Gray• Iron• Lava• Rainbow• Rainbow HC |
| Set-up commands | Date/time, Temperature (°C/°F) |
| Web interface | Yes |
| Storage of images | |
| Storage media | Built-in memory for image storage |
| Image storage mode | IR, visual, MSX |
| File formats | JPEG + FFF |
| Image streaming | |
| Image streaming formats | <ul style="list-style-type: none">• Motion JPEG stream MJPEG Baseline Process Encoder Baseline ISO/IEC 10918-1 JPEG compliance• MPEG stream Stream format MPEG-4 ISO/IEC 14496-2 Simple Profile level 2• H.264 stream Stream format H.264 Baseline Profile level 2.0 |
| Image streaming resolution | 640 × 480 |
| Image modes | <ul style="list-style-type: none">• Thermal• Visual• MSX |
| Automatic image adjustment | Continuous |
| Multi Spectral Dynamic Imaging (MSX) | IR image with enhanced detail presentation |
| Ethernet | |
| Ethernet | Control, result and image |
| Ethernet, type | 100 Mbps |
| Ethernet, standard | IEEE 802.3 |
| Ethernet, connector type | M12 8-pin X-coded |
| Ethernet, communication | TCP/IP socket-based FLIR proprietary |
| Ethernet, video streaming | Yes |
| Ethernet, power | Power over Ethernet, PoE IEEE 802.3af class 2. |
| Ethernet, protocols | Ethernet/IP, Modbus TCP, TCP, UDP, SNTP, RTSP, RTP, HTTP, ICMP, IGMP, sftp, SMTP, DHCP, MDNS (Bonjour) |
| Digital input/output | |
| Digital input, purpose | NUC, NUC disable, Alarm |
| Digital input | 1 opto-isolated, 10–25 VDC |
| Digital output, purpose | As function of alarm, output to ext. device (programmatically set) |
| Digital output | 1 opto-isolated, 10–25 VDC, max. 100 mA |
| Digital I/O, isolation voltage | 500 VRMS |
| Digital I/O, supply voltage | 10–25 VDC, max. 200 mA |
| Digital I/O, connector type | M12 8-pin A-coded (shared with ext. power) |

P/N: 71201-0101

© 2023, FLIR Systems, Inc.
#71201-0101; r. 81601;

| Power system | |
|----------------------------------|---|
| External power operation | 12/24 VDC, 2 W continuously/ 4.7 W absolute max |
| External power, connector type | M12 8-pin A-coded (Shared with digital I/O) |
| Voltage | Allowed range 10.8–30 VDC |
| Power supply rating | Class 2 / LPS |
| Environmental data | |
| Operating temperature range | -0°C to +50°C (+32°F to +122°F) |
| Storage temperature range | -40°C to +70°C (-40°F to +158°F) according to IEC 68-2-1 and IEC 68-2-2 |
| Humidity (operating and storage) | IEC 60068-2-30/24 h 95% relative humidity +25°C to +40°C (+77°F to +104°F)/ 2 cycles |
| EMC | <ul style="list-style-type: none"> • EN 61000-6-2:2001 (Immunity) • EN 61000-6-3:2001 (Emission) • FCC 47 CFR Part 15 Class B (Emission) |
| Encapsulation | IP 67 (IEC 60529) |
| Bump | 25 g (IEC 60068-2-29) |
| Vibration | 2 g (IEC 60068-2-6) |
| Declaration of conformity | See: https://support.flir.com/resources/DoC |
| Physical data | |
| Weight | 0.125 kg (0.28 lb.) |
| Camera size (L × W × H) | <ul style="list-style-type: none"> • 54 × 25 × 79 mm (2.1 × 1 × 3.1 in.) without connectors • 54 × 25 × 95 mm (2.1 × 1 × 3.7 in.) with connectors |
| Base mounting | 4x mounting hole depth max 4.8 mm for screw type Delta PT 22 (ø2.2 mm) |
| Housing material | PA6 with 30% GF (glass fiber reinforced) |
| Shipping information | |
| Packaging, type | Cardboard box |
| List of contents | <ul style="list-style-type: none"> • Infrared camera with lens • Cardboard box • Printed documentation |
| Packaging, weight | 0.48 kg (1.06 lb.) |
| Packaging, size | 210 × 142 × 70 mm (8.27 × 5.59 × 2.76 in.) |
| EAN-13 | 4743254001725 |
| UPC-12 | 845188009373 |
| Country of origin | Estonia |

Supplies & accessories:

- T131367; FLIR Bridge
- T131369; FLIR Bridge Pro
- T130086; I/O module MIO-AX8-1
- T130087; I/O module MIO-AX8-7
- T199713; ThermoVision CM Panel, max. 4 cameras
- T199712; ThermoVision CM Panel, max. 9 cameras
- T130169; Thermovision CM, max. 4 cameras
- T130170; Thermovision CM, max. 9 cameras
- T129259ACC; Cable M12 to pigtail, 10 m



FLIR AX8 9 Hz

P/N: 71201-0101

© 2023, FLIR Systems, Inc.


#71201-0101; r. 81601;

- T129258ACC; Cable M12 to pigtail, 5 m
- T129886ACC; Cable M12, FLIR X-Coded to standard X-Coded
- T128391ACC; Cable, M12 to pigtail
- T198821; Cooling bracket
- T129257ACC; Ethernet cable M12 to RJ45, 10 m
- T128390ACC; Ethernet cable M12 to RJ45, 2 m
- T129256ACC; Ethernet cable M12 to RJ45, 5 m
- 71200-0002; FLIR AX8 accessory starter kit
- T199163; Front mounting plate kit (incl. cooling bracket)
- T199342; One-ball joint mounting bracket kit
- T199343; PoE injector, 12/24 V
- T128775ACC; Rear mounting plate kit
- T199341; Two-ball joint mounting bracket kit

This technical drawing provides three views of the FLIR AX-Series camera: Front View (A), Top View (B), and Side View (C). The drawing includes detailed dimensions for each view and callouts pointing to specific features.

- Front View (A):** Shows the camera from the front. Dimensions include height [0.39], width [9.9 ±0.02], depth [0.5 ±0.01], and mounting hole depth [20 ±0.5].
- Top View (B):** Shows the camera from above. Dimensions include height [0.79 ±0.02], width [2.16 ±0.04], depth [55 ±0.1], and mounting hole depth [1.57 ±0.08].
- Side View (C):** Shows the camera from the side. Dimensions include height [1.45 ±0.00], width [36.8 ±0.1], depth [25.6 ±0.5], and mounting hole depth [4x Mounting hole depth max 4,8 mm for screw type Delta PT 22 (ø2,2 mm)].
- Callouts:**
 - Front View Callout:** Points to the Power / Error indicator (Blue / Red) and the Ethernet communication indicator (Green).
 - Top View Callout:** Points to the Reset button, Ethernet communication indicator (Green), and the Power / Error indicator (Blue / Red).
 - Side View Callout:** Points to the Power/I/O connector M12/8A, the Ethernet connector M12/8X, the Visual camera, and the IR sensor.
- Annotations:**
 - According to following P/N numbers:**
 - 71201-0101
 - 71202-0201
 - E70321
 - Basic dimensions AX-series:** A table listing basic dimensions for the AX-Series.
 - FLIR Logo:** Located in the top right corner.


This document must not be copied completely or in part.
Any infringement will be illegal.

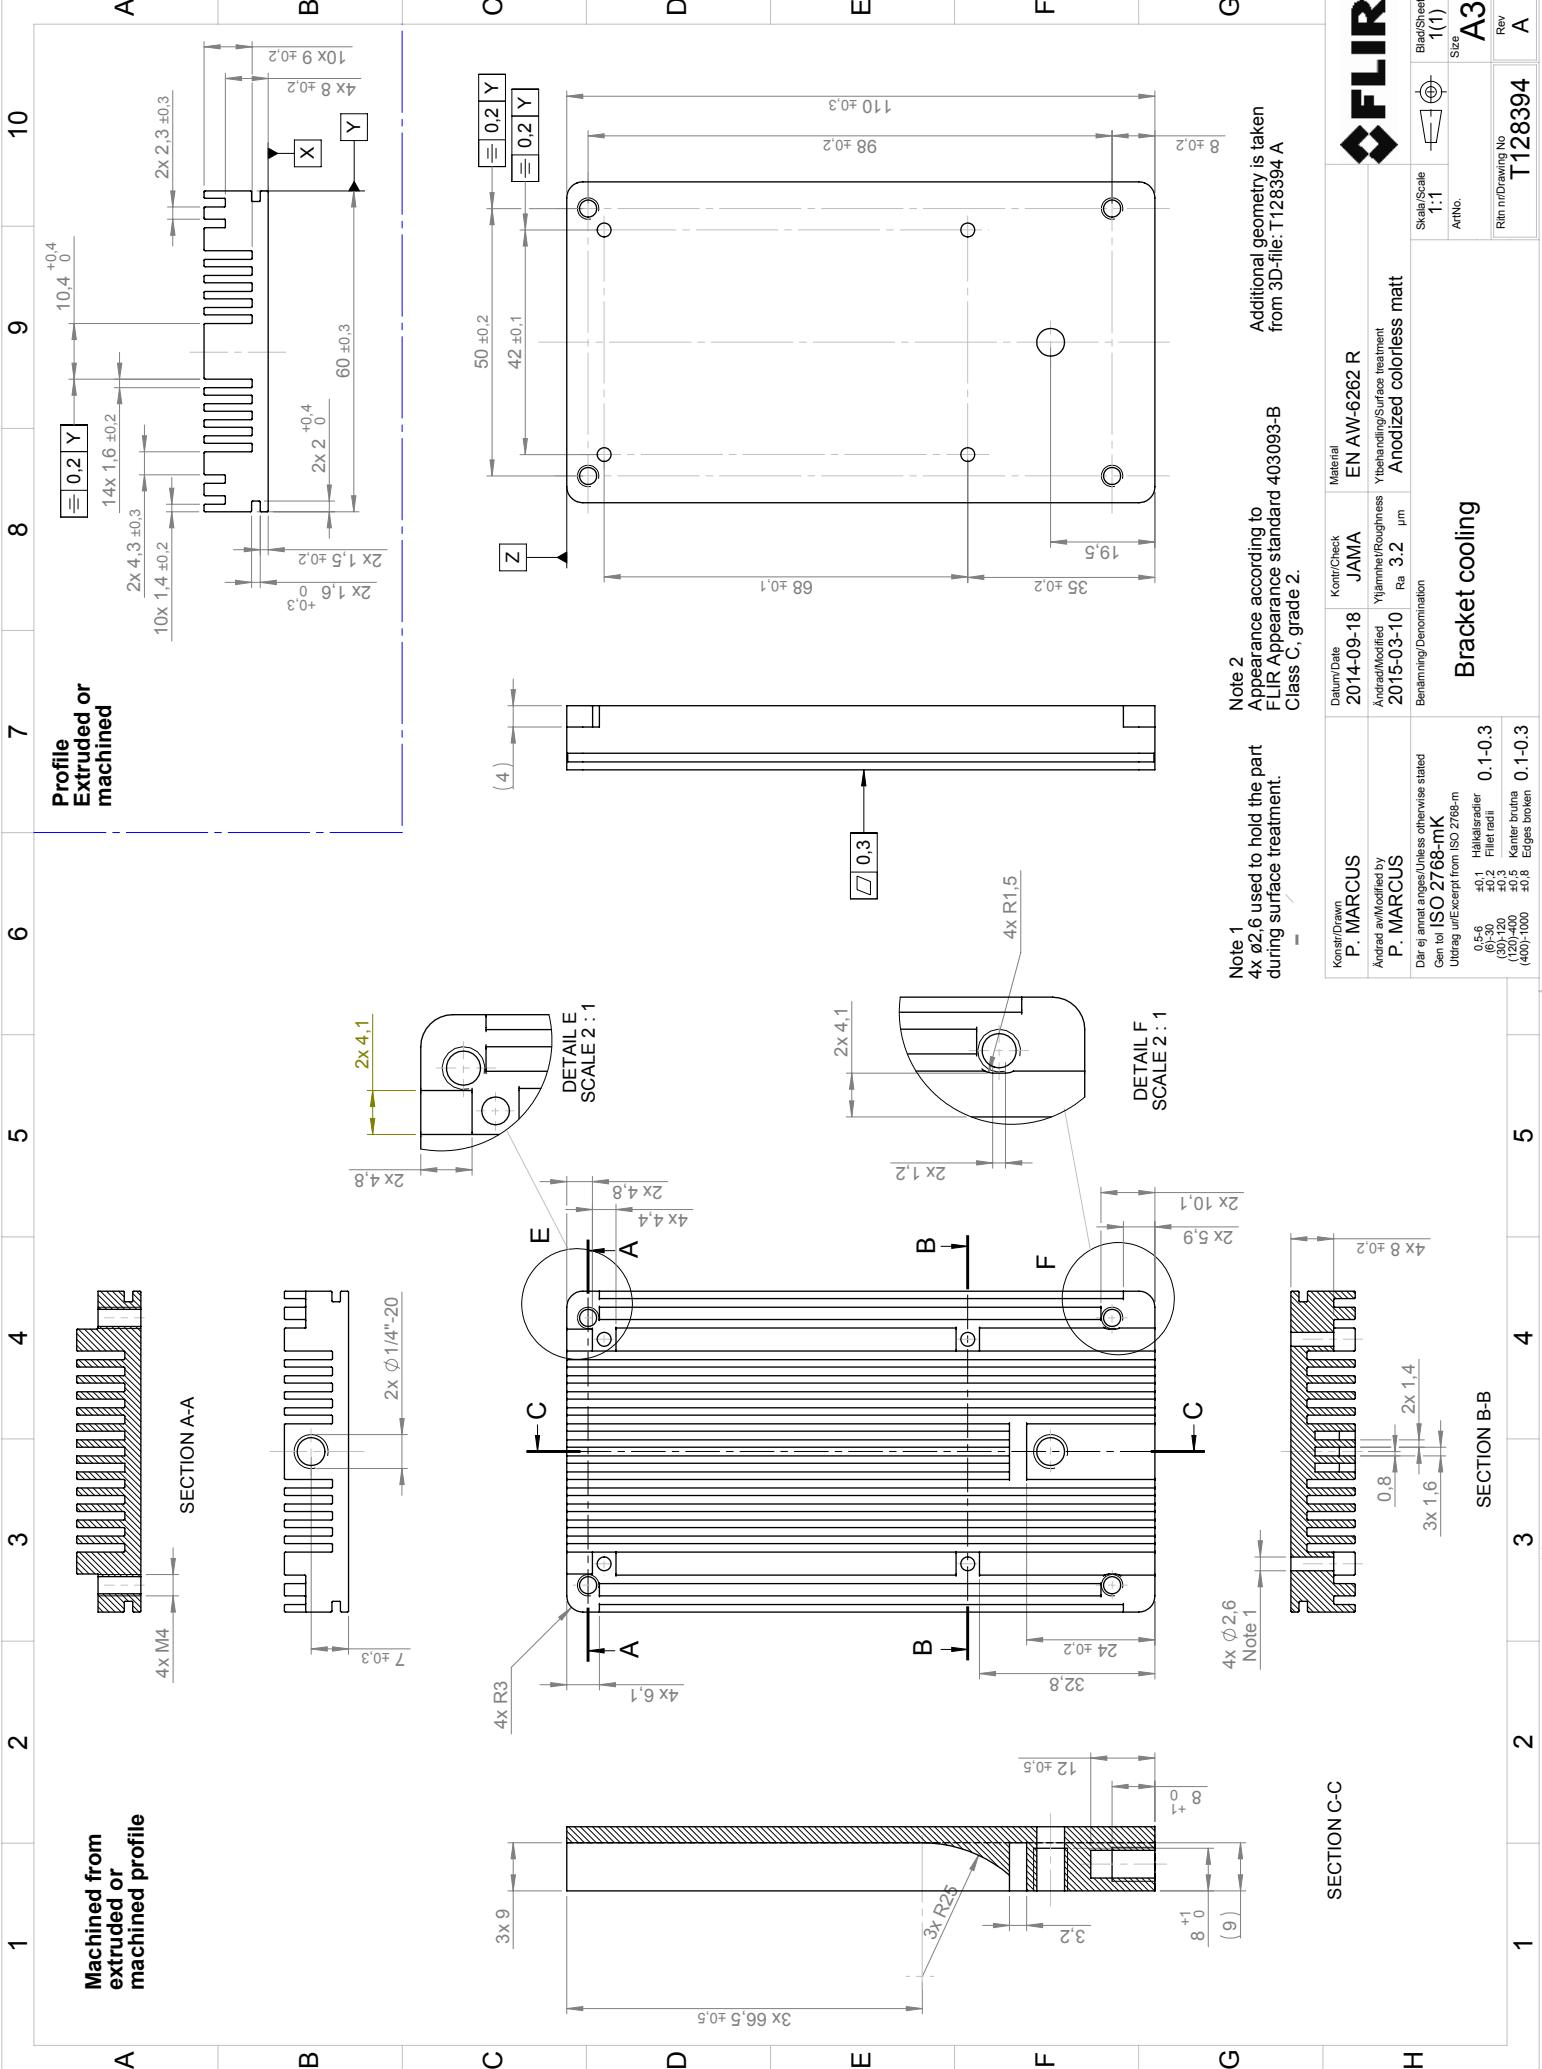


FLIR SYSTEMS AB
Den enklaste teknik för att identifiera härliga detaljer med stor noggrannhet.
Detta dokument måste inte tas tillbaka om det är kopierat i delar.


FLIR SYSTEMS AB
Any infringement will lead to legal proceedings.
Copied completely or in part without our permission.
This document must not be communicated outside the company.

| | |
|---------------------------|-----------------|
| FLIR® | Size A3 |
| Rev A | Blad/Sheet 1(1) |
| Ref nr/Drawing No T128394 | ArtNo. |
| 1(1) | Scale/Scale 1.1 |

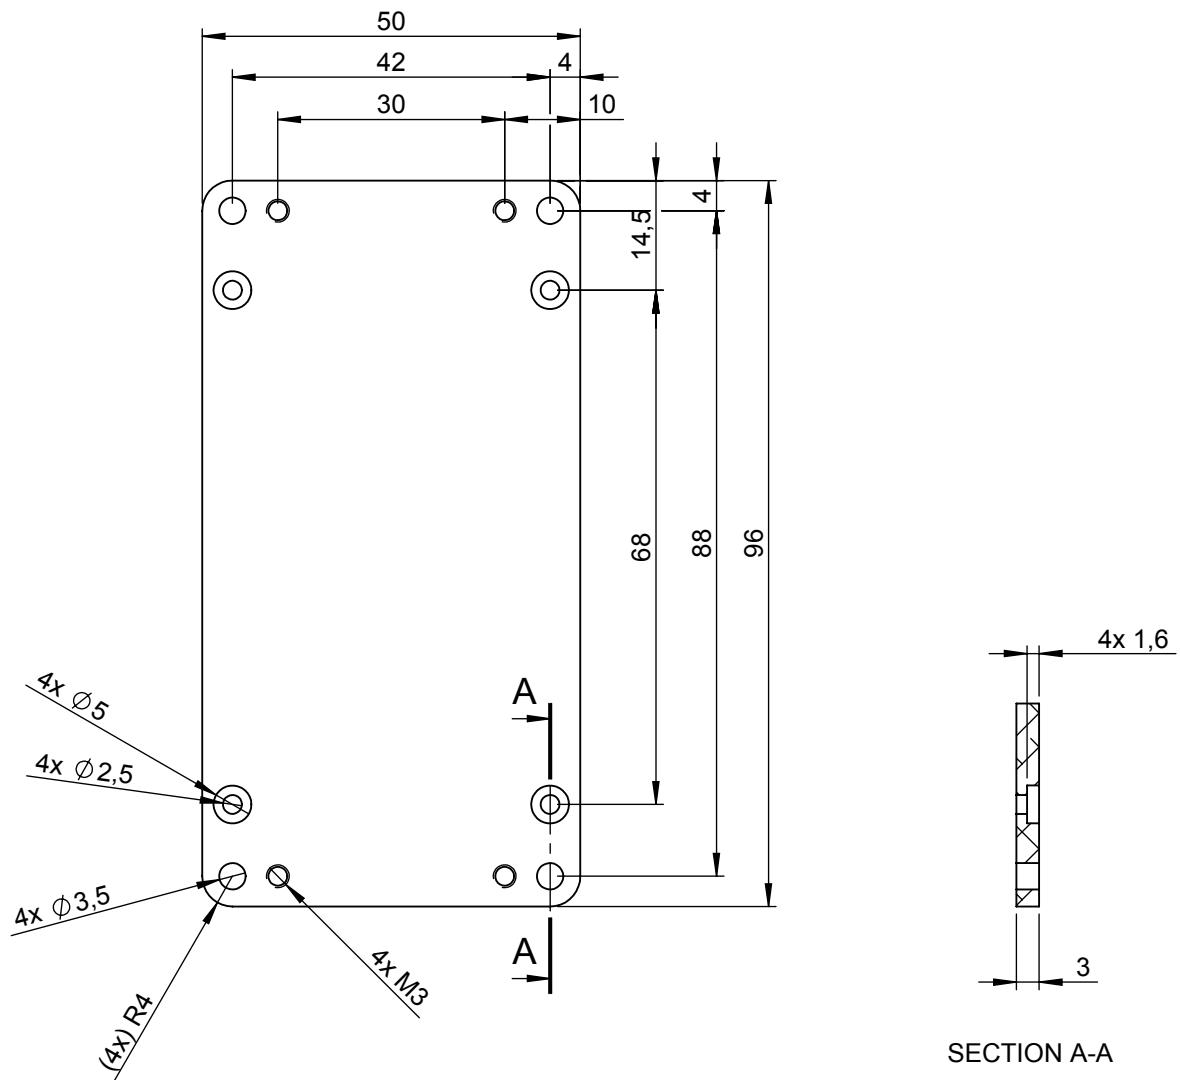


SECTION A-A

| | | | | |
|--|--|---|---|---|
| Konstr/Drawn J. MÄKINEN | Datum/Date 2015-03-06 | Kontroll/Check HAOS | Material EN AW-5052 or EN AW-5754 |  |
| Ändrad av/Modified by J. MÄKINEN | Ändrad/Modified 2015-05-21 | Ytjämnhet/Roughness Ra μm | Ytbehandling/Surface treatment | |
| Där ej annat anges/Unless otherwise stated Gen tol ISO 2768-mK Utdrag ur/Excerpt from ISO 2768-m | Benämning/Denomination Plate mounting rear | | | |
| 0,5-6 $\pm 0,1$ Hålkärlsradii (6)-30 $\pm 0,2$ Fillet radii (30)-120 $\pm 0,3$ (120)-400 $\pm 0,5$ Kanter brutna (400)-1000 $\pm 0,8$ Edges broken | Skala/Scale 1:1 | |  | Blad/Sheet 1(1) |
| | Art.No. | | | Size A4 |
| | Ritn nr/Drawing No T128775 | | | Rev A |


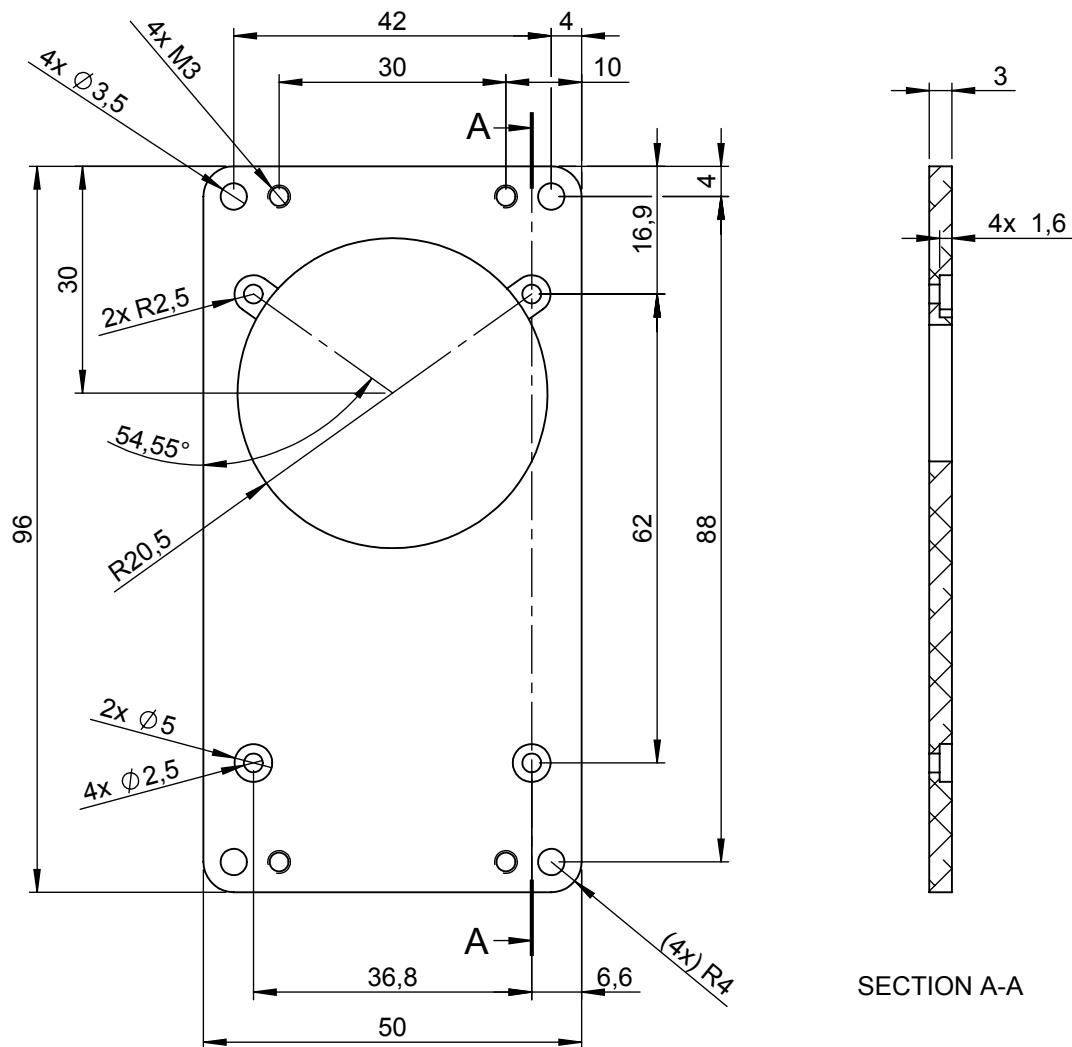


SECTION A-A

| | | | | |
|---|---|---|---|---|
| Konstr/Drawn J. MÄKINEN | Datum/Date 2015-03-06 | Kontroll/Check HAOS | Material EN AW-5052 or EN AW-5754 |  |
| Ändrad av/Modified by J. MÄKINEN | Ändrad/Modified 2015-05-21 | Ytjämnhet/Roughness Ra μm | Ytbehandling/Surface treatment | |
| Där ej annat anges/Unless otherwise stated Gen tol ISO 2768-mK Utdrag ur/Excerpt from ISO 2768-m | Benämning/Denomination Plate mounting front | | | |
| 0,5-6 $\pm 0,1$ Hälkärsradijer (6)-30 $\pm 0,2$ Fillet radii (30)-120 $\pm 0,3$ (120)-400 $\pm 0,5$ Kanter brutna (400)-1000 $\pm 0,8$ Edges broken | Skala/Scale 1:1 | |  | Blad/Sheet 1(1) |
| | Art.No. | | | Size A4 |
| | Ritn nr/Drawing No T128774 | | | Rev A |

RoHS 
IP67

| REV. | DESCRIPTION | DATE |
|------|-------------------------------------|-------------|
| A | ISSUE | Dec/23/2013 |
| B | Modify the wire diagram. | Dec/25/2013 |
| C | Modify M12 Pin Assignment. | Dec/25/2013 |
| D | Modify cable length. | Dec/25/2013 |
| D1 | Correct key direction. | Jan/22/2014 |
| E | Add note. | Mar/30/2014 |
| F | Modify P/N. | Sep/25/2014 |
| G | Modify connector to shielding type. | Nov/12/2014 |
| G1 | Change ring nut to shielding type. | Nov/25/2014 |


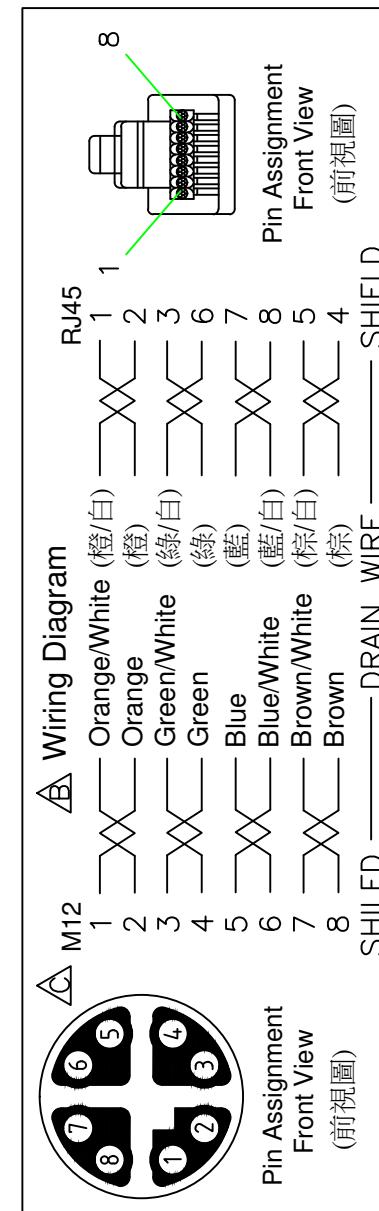
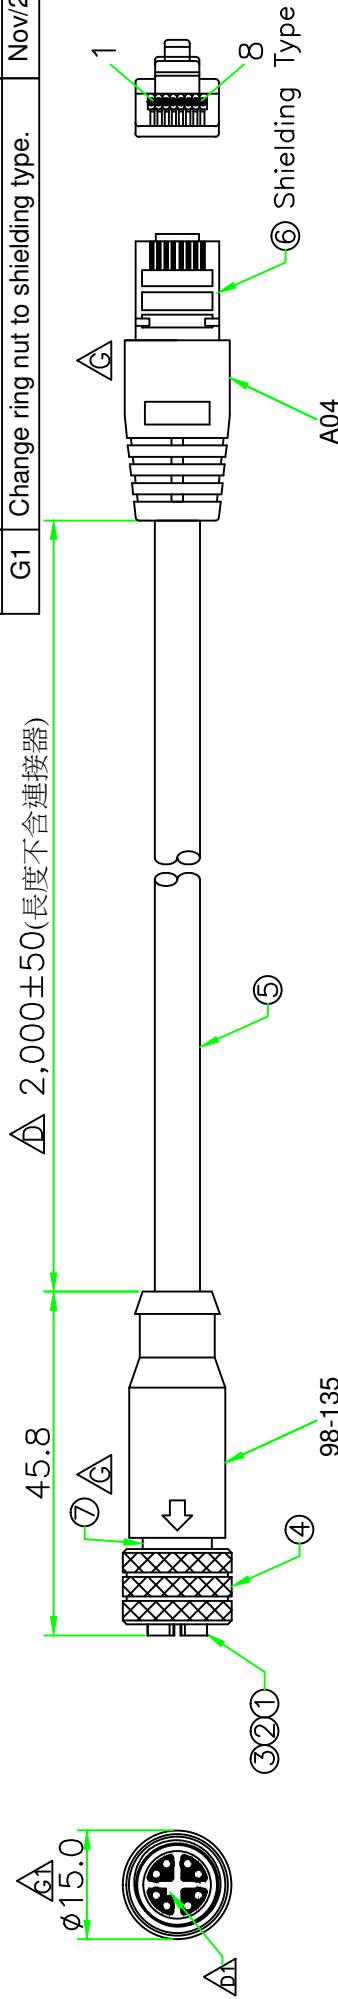


| No. | PART NAME | DESCRIPTION | COLOR | Q'TY | REMARKS | DWG.NO: | | |
|-----|-----------|---|-------|------|----------------|--|-----------------|---------------------------------------|
| | | | | | | G1 | 1/1 | AP. |
| 7 | SHIELD | Brass, Nickel Plated. | | | | 1 | | |
| 6 | RJ45 PLUG | RJ45 8P8C PLUG (shielding type). | | | | 1 | | |
| 5 | CABLE | CAT5E FTP 24AWG x 4 PAIR + AL/MY + Drain wire. | BLACK | 1 | WAC2B0026 | | | |
| 4 | RING NUT | Brass, Nickel Plated. | BLACK | 1 | M12S-RN-D965 | | UNIT:mm | M12 X-Coding Female Molded Cable Assy |
| 3 | O-RING | Viton. | BLACK | 1 | M12-O-VK | SCALE | 1:1 | |
| 2 | CONTACT | Brass, Female pin ,6 u" Gold plated . | | 8 | AASPF-1008-0.8 | UNLESS OTHERWISE SPECIFIED TOLERANCES: x ± 0.25 mm xxx ± 0.05 mm ANGLE ± 1° | P/N: K129351004 | DR. Stanley |
| 1 | CONNECTOR | M12 X-coding Female connector insert. Nylon+GF. | BLACK | 1 | M12X-08F | REV. SHEET | CH. ERIC | AP. |

Customer: FLIR

RoHS  **IP67**

| REV. | DESCRIPTION | DATE |
|------|-------------------------------------|-------------|
| A | ISSUE | Dec/23/2013 |
| B | Modify cable length. | Dec/25/2013 |
| C | Add note. | Mar/20/2014 |
| D | Modify P/N. | Sep/25/2014 |
| E | Modify connector to shielding type. | Nov/12/2014 |
| E1 | Change ring nut to shielding type. | Nov/25/2014 |

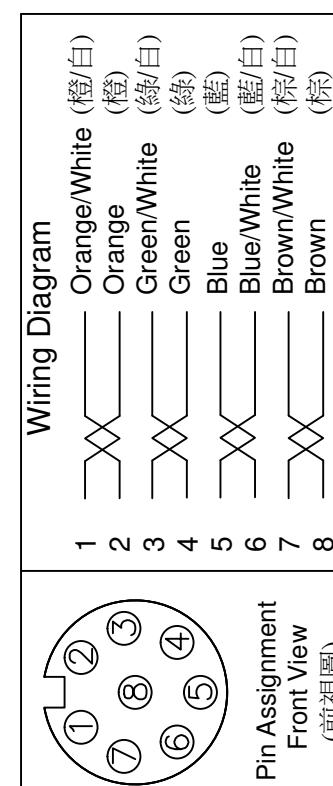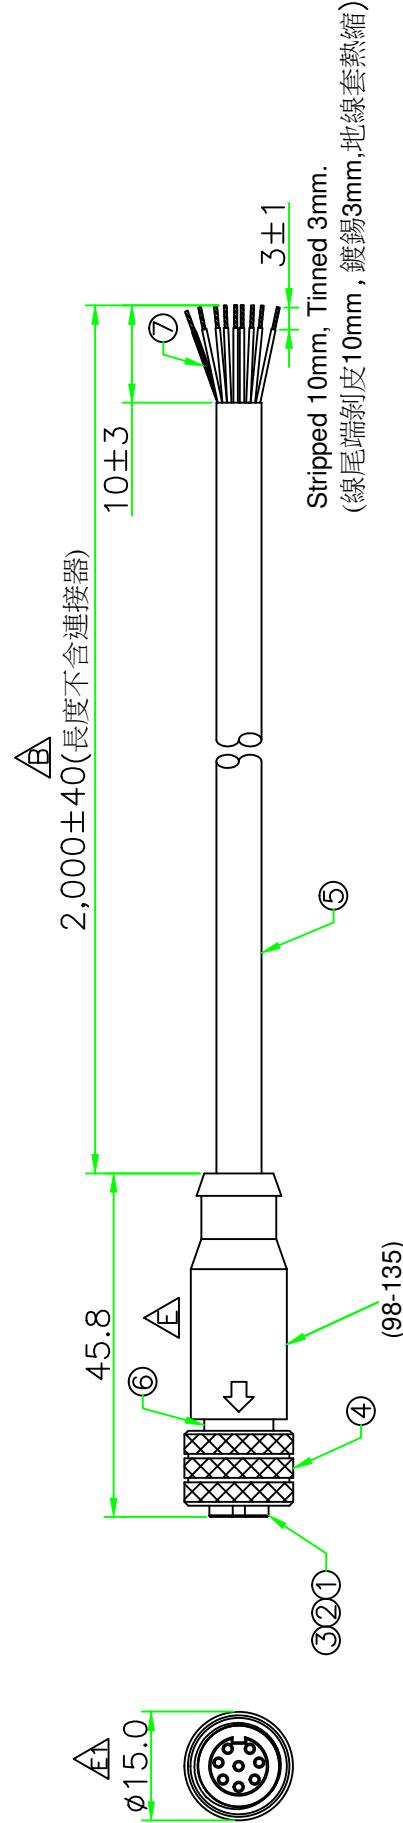


| 7 | TUBE | Heat shrink tube. | BLACK | 1 | Customer: FLIR | |
|-----|-----------|---|-------|------|---|---|
| 6 | SHIELD | Brass, Nickel Plated.  | | 1 | | |
| 5 | CABLE | CAT5E FTP 24AWG x 4 PAIR + AL/MY + Drain wire. | BLACK | 1 | WAC2B0026 | |
| 4 | RING NUT | Brass, Nickel Plated. | | 1 | M12S-RN-D865 |  UNIT:mm |
| 3 | O-RING | Viton. | BLACK | 1 | M12-O-VK | SCALE 1:1 |
| 2 | CONTACT | Brass, Female pin ,6 u" Gold plated . | | 8 | AASPF-1008-0.8 x ± 0.25 xx ± 0.1 xxx ± 0.05 ANGLE ± 1°X | UNLESS OTHERWISE SPECIFIED TOLERANCES: P/N: K129351003 |
| 1 | CONNECTOR | M12 A-coding Female connector insert. Nylon+GF. | BLACK | 1 | M12A-08F | REV. SHEET |
| No. | PART NAME | DESCRIPTION | COLOR | Q'TY | REMARKS | DWG.NO: T128391  |


AP.

ERJC

Stanley

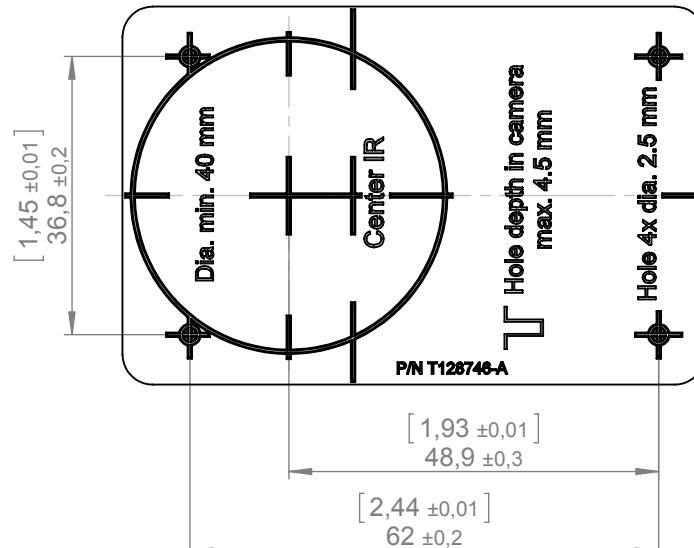


Scale 1:1

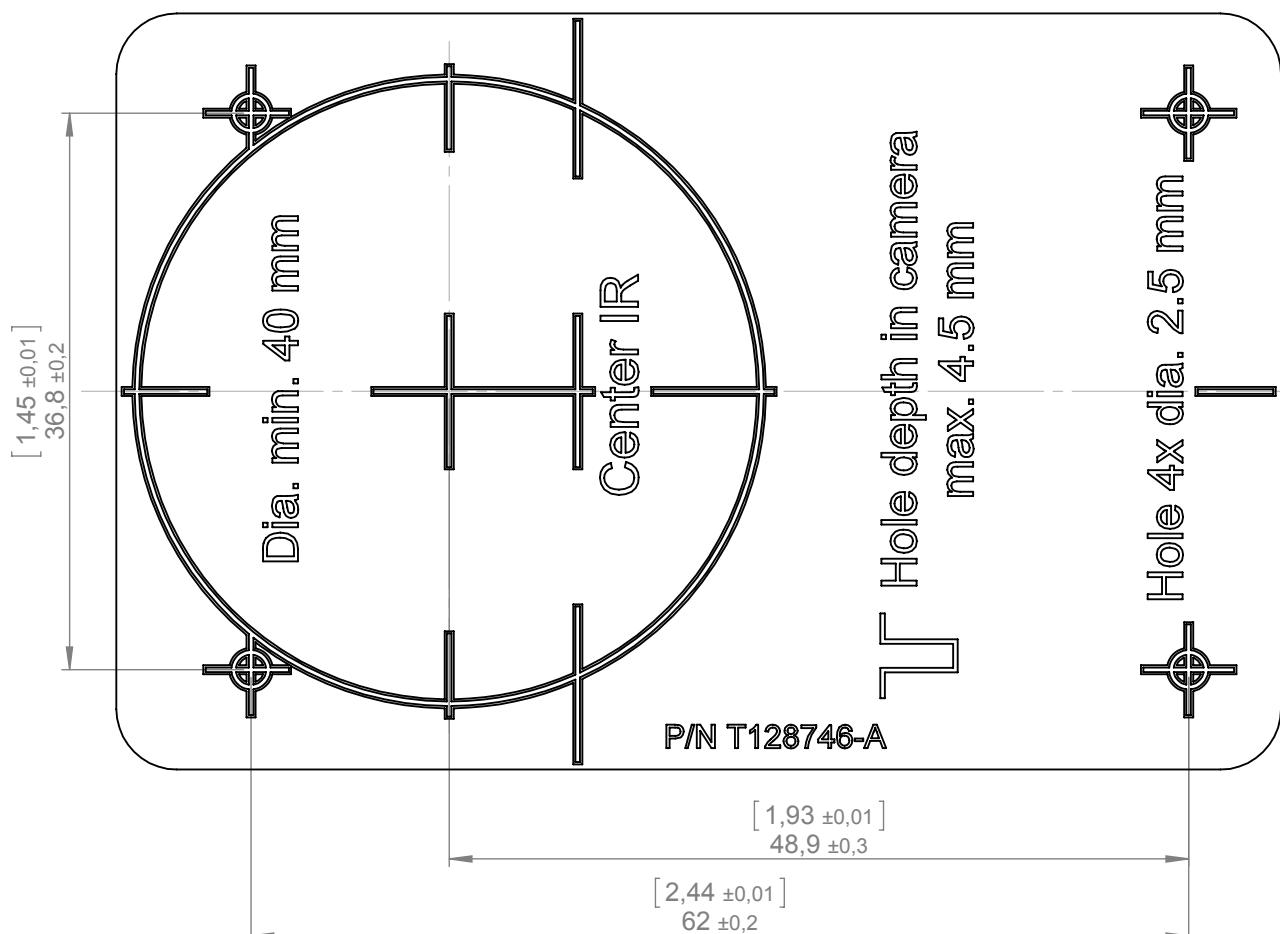


Scale 2:1

| | | | | |
|---|--------------------------------------|--|--------------------------------------|---------------------------|
| Konstr/Drawn P. MARCUS | Datum/Date 2014-10-06 | Kontroll/Check JAMA | Material Note 1 | FLIR |
| Ändrad av/Modified by P. MARCUS | Ändrad/Modified 2015-03-04 | Ytjämnhet/Roughness Ra μm | Ytbehandling/Surface treatment | |
| Där ej annat anges/Unless otherwise stated Gen tol ISO 2768-mK | Benämning/Denomination | | | |
| Utdrag ur/Excerpt from ISO 2768-m | Drilling template front | | | |
| 0,5-6 (6)-30 (30)-120 (120)-400 (400)-1000 | ±0,1 ±0,2 ±0,3 ±0,5 ±0,8 | Hålkärlsradii Fillet radii Kanter brutna Edges broken | Skala/Scale 2:1 | Blad/Sheet 2(2) |
| | | | Art.No. | Size A4 |
| | | | Ritn nr/Drawing No T128746 | Rev A |

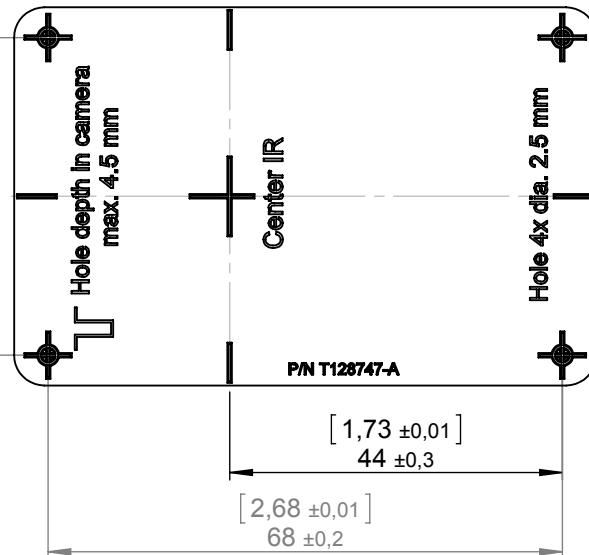

Scale 1:1

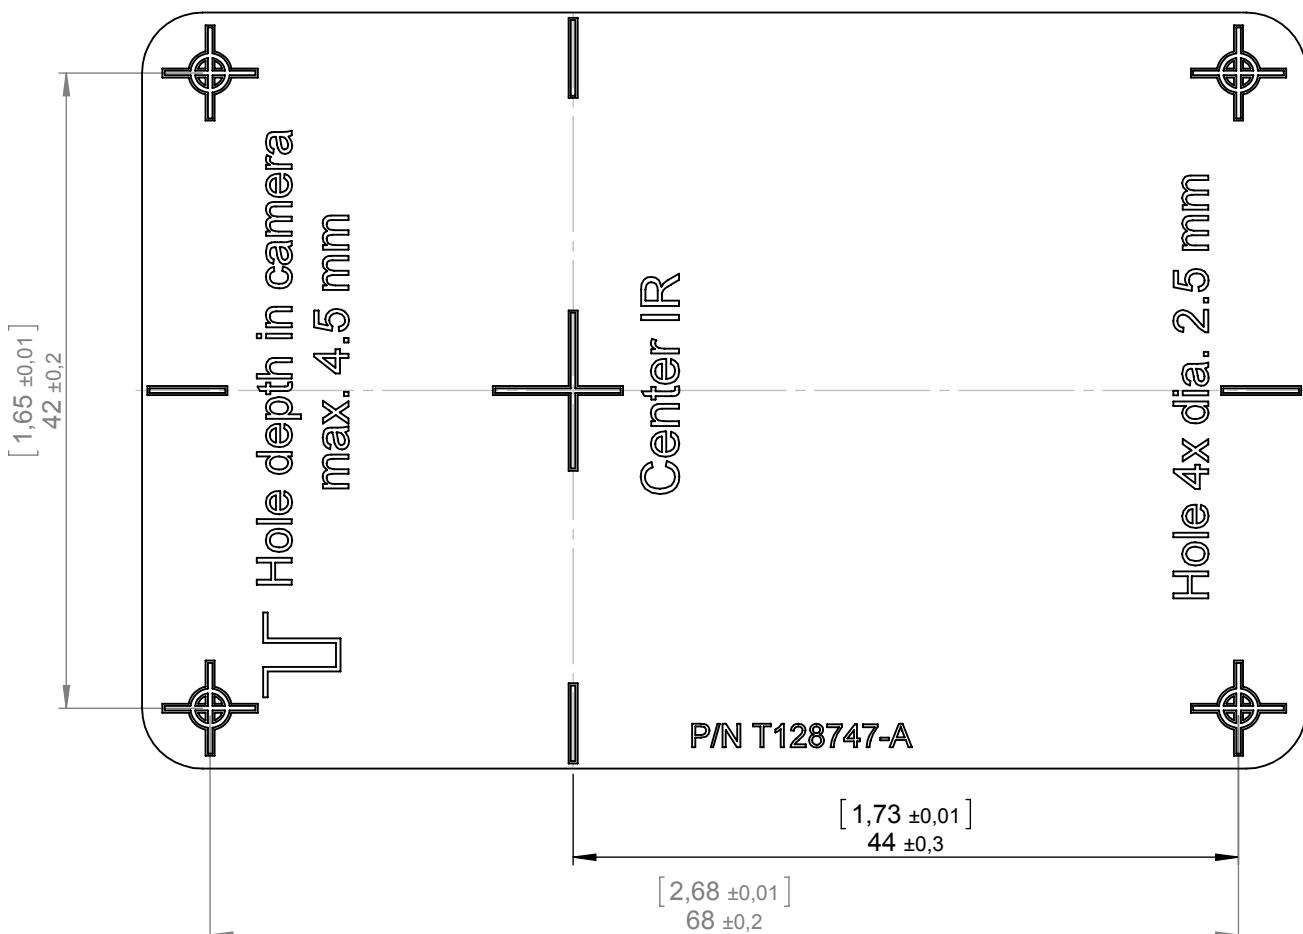

Scale 2:1

| | | | | |
|--|--------------------------------------|-----------------------------------|--------------------------------|---|
| Konstr/Drawn P. MARCUS | Datum/Date 2014-10-06 | Kontroll/Check JAMA | Material Note 1 |  |
| Ändrad av/Modified by P. MARCUS | Ändrad/Modified 2015-03-04 | Ytjämnhet/Roughness Ra µm | Ytbehandling/Surface treatment | |
| Där ej annat anges/Unless otherwise stated Gen tol ISO 2768-mK | Benämning/Denomination | | | Skala/Scale 2:1 |
| Utdrag ur/Excerpt from ISO 2768-m | Drilling template rear | | | Blad/Sheet 2(2) |
| 0,5-6 ±0,1 Hålkärsradier (6)-30 ±0,2 Fillet radii (30)-120 ±0,3 (120)-400 ±0,5 Kanter brutna (400)-1000 ±0,8 Edges broken | Art.No. | | Size A4 | Rev A |
| | Ritn nr/Drawing No T128747 | | | |

Digital I/O connection diagrams FLIR AX8

