



SFS01 EvaKit



Thermal mass flow sensor Optimal for demonstration and evaluation of the SFS01 (Silicon Flow Sensor)



Benefits & Characteristics



Characteristics


- Measurement from 0 to 200 sccm
- Detection of flow direction
- Analog and digital (I²C) connection
- Pneumatic connections for gas


Applications


- Automation technology
- Process and regulation technology
- Medicinal and biological technology
- Air conditioning
- Battery-operated applications in portable devices

Illustration

Illustration and dimensions (in mm) of the SFS chip

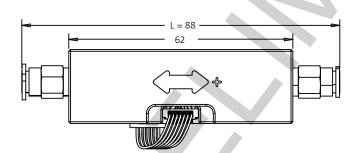



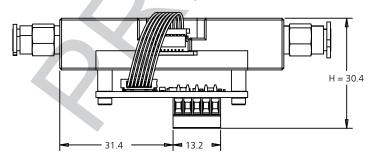

1) For exact size see measurements













Technical Data

| Integrated sensor: | SFS01 |
|---------------------------------|---|
| Dimensions (L x W x H): | 88.0 (±0.5) x 27.5 (±1.0) x 30.4 (±0.5) |
| Channel dimensions (L x W x H): | 35.0 (±0.15) x 1.0 (±0.05) x 1.0 (±0.05) |
| Pneumatic connections: | QSM M5-4 |
| Temperature range: | 0 °C to +80 °C |
| Storage temperature: | -20 °C to +80 °C |
| Pressure load: | Up to 1 bar (one-sided on membrane over 10 years) |
| | |

Product Photo



Electrical Data

| Supply voltage: | 5 ± 5% V |
|---------------------|---|
| Power: | Typ 30 mW |
| Output voltage: | 0 to 5 V, ca. 2.5 ±0.2 V at 0 sccm |
| Digital connection: | 3.3 V I ² C (pull up resistors on board) |
| Digital signal: | Calibrated signal (up to ±200 sccm) Raw signal (digits) |
| Analog output load: | < 1 mA |

Flow Performance

The following values are viewed as typical and achieved in laboratory conditions. The gas used was nitrogen.

| Medium: | non-aggressive gases (5-95 % rel. humidity, non-condensing) |
|---------------------------------|---|
| Measurement range: | 0 to ±200 sccm |
| Sensitivity: | 0.1 sccm |
| Response time t ₆₃ : | 10 ms |
| Accuracy: | 3.0 % F.S. |
| Temperature sensitivity: | < 0.25 %/K F.S. |

SFS01 EvaKit | Flow | SFS01 EvaKit
















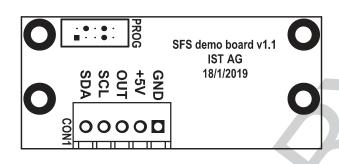


| 1 | 2 | 3 | 4 | 5 |
|-------------|--------------|--------|----------------|--------|
| SDA | SCL | OUT | +5V | GND |
| Serial Data | Serial Clock | Output | Supply voltage | Ground |

I²C Protocol

I²C Protocol Description

For integration with a micro-controller, the SFS Demo Board has an I²C-compatible interface which supports both 100 kHz and 400 kHz bit rates. The default I²C slave address is programmed on 0x28 and can be adjusted in the entire 7-bit address range (0x00 to 0x7F).

| Paramet | ter | min | max | unit |
|---------------------|---|-----|-----|------|
| f _{SCL} | SCL clock frequency | 100 | 400 | kHz |
| t _{HD,STA} | Hold time (repeated) START | 0.6 | | μs |
| t _{su,sta} | Setup time for a repeated START | 0.6 | | μs |
| t _{HD,DAT} | Data hold time | 0 | | μs |
| t _{SU,DAT} | Data setup time | 250 | | μs |
| t _{su,sto} | Setup time for STOP | 0.6 | | μs |
| t _{sp} | Pulse duration of spikes suppressed by input filter | 50 | 600 | ns |

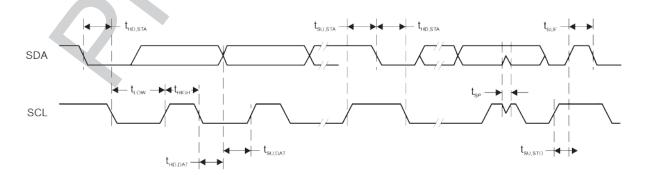













Reading the data form SFS Demo Board

During normal operation the SFS Demo Board is ready to transmit current calibrated and raw flow's value. The typical transmission is:

Start | Address | R | ACK | Data[0] | ACK | Data[1] | ACK | Data[2] | ACK | Data[3] | ACK | Stop

Start | Address | R | ACK | Data[0] | ACK | Data[1] | ACK | Stop

| Data | | Parameter | Unit | |
|----------|-------------|------------------|------|--|
| Data [0] | higher bite | Calibrated flow | cccm | |
| Data [1] | lower bite | Calibrated flow | sccm | |
| Data [2] | higher bite | Raw flow value | | |
| Data [3] | lower bite | Navv 110vv value | | |

The calibrated flow read from the module is in signed fixed-point integer Q6 format. To convert it to decimal format, the read value has to be divided by $2^6 = 64$. The minimum value is -512, the maximum value is 511.98438. The resolution of each value is $1/2^6 = 0.015625$. The raw value read from the module is in unsigned integer format.

| MSB | | | | | | | | | | | LSB |
|-------|--------------|--|--|--|--|--|---|--------|---------|----|-----|
| 30 00 | Integer bits | | | | | | F | ractio | nal bit | 15 | 3 |

Entering the Command Mode

To read, write parameters or remote-reboot, the SFS Demo Board must be set to command mode by writing 0xA0.

| C++ | A -l -l | 107 | A C 1/ | D-+- 040 | A C 1/ | CTOD |
|-------|---------|-----|--------|-------------|--------|------|
| Start | Address | W | ACK | Data = UXAU | ACK | STOP |

In the command mode the SFS Demo Board switches off flow's measurement and waits for further communication. The module will reboot automatically after 0.5 second of idle or unsuccessful transmission. The module requires up to 1 ms for entering the command mode (counted from stop bit).

Entering the Command

In the command mode the user can transmit a 1-byte instruction to the module. The module requires up to 1 ms to process the instruction.

| Start | Address | W | ACK | Data = Instruction's code | ACK | STOP |
|-------|--------------------------|----------|------------|--------------------------------|-----|------|
| 0.00 | 1.50 | 1:1 | | | | |
| 0x00: | | | • | arameter (do not change!) | | |
| 0x01: | read Flow B | calibr | ation's p | arameter (do not change!) | | |
| 0x02: | read Flow C | calibr | ation's p | arameter (do not change!) | | |
| 0x03: | read Flow D | calibr | ation's p | arameter (do not change!) | | |
| 0x04: | read Flow's | Range | | | | |
| 0x05: | read I ² C_ad | ldress - | own ac | ddress on I ² C bus | | |
| 0x06: | read Serial I | Numbe | er | | | |
| 0x07: | read Firmw | are Rev | /ision | | | |
| 0x20: | write Flow | A calib | ration's p | parameter (do not change!) | | |
| 0x21: | write Flow I | B calib | ration's p | parameter (do not change!) | | |
| 0x22: | write Flow | C calib | ration's p | parameter (do not change!) | | |
| 0x23: | write Flow I | D calib | ration's p | parameter (do not change!) | | |
| 0x24: | write Flow's | Range | 9 | | | |
| 0x25: | write I ² C_a | ddress | – own a | ddress on I ² C bus | | |
| 0xa1: | exit comma | nd mo | de (with | out reset) | | |
| 0xa2: | reboot | | | | | |













Reading parameters from the module

After successful read instruction the module fills the I²C buffer with the selected parameter. All parameters read from the module, except I²C_address, Serial Number and Firmware Revision, are in signed fixed-point long IQ22 format (4 bytes). To convert them to decimal format the read value has to be divided by $2^{22} = 4194304$. The minimum value is -512, the maximum value is 511.999 999 762. The resolution of each parameter is $1/2^{22} = 0.0000000238$. I²C_address, Serial Number and Firmware Revision parameters are read in unsigned long format. Additionally, I²C_address is internally masked with 0x3ff.

| Start | Address | R | ACK | Data[3] | ACK | Data[2] | ACK | 1.46 | Data[0] | ACK | Stop | |
|-------|---------|---|-----|---------|-----|---------|-----|------|---------|-----|------|--|
|-------|---------|---|-----|---------|-----|---------|-----|------|---------|-----|------|--|

| Da | ata | Parameter |
|----------|-----------------------------------|-----------|
| Data [3] | 1 st byte (highest) | |
| Data [2] | 2 nd byte | Parameter |
| Data [1] | 3 rd byte | Parameter |
| Data [0] | 4 th byte (lowest) | |

After transmitting 4 bytes, the module resets the internal timer and waits in command mode for the next command. The module will reboot automatically after 0.5 second of idle or unsuccessful transmission.

Writing parameters to the module

After successful write instruction the module waits for 4 bytes with the new parameter. All parameters except I²C_address, Serial Number and Firmware Revision written to the module are in signed fixed-point long IQ22 format (4 bytes). In order to convert decimal format to IQ22, the decimal value has to be multiplied by 2²² = 4 194 304. To reduce the error, this calculation should be done as double precision floating point number. The minimum value is -512, the maximum value is 511.999 999 762. The resolution of each parameter is 1/2²² = 0.000 000 238. I²C_address, Serial Number and Firm-ware Revision parameters are written in unsigned long format. Additionally, I²C_address is internally masked with 0x3ff. Please mind that the new I²C address applies after reboot. The module requires up to 1 ms after stop bit to flash the internal memory with the new parameter.

| Start Address V | W ACK Data[3] | ACK Data[2] | ACK | Data[0] | ACK Stop |
|-----------------|---------------|-------------|-----|---------|----------|

| Da | ata | Parameter |
|----------|-----------------------------------|-----------|
| Data [3] | 1 st byte (highest) | |
| Data [2] | 2 nd byte | Daramatar |
| Data [1] | 3 rd byte | Parameter |
| Data [0] | 4 th byte (lowest) | |

After receiving 4 bytes, the module resets the internal timer and waits in command mode for the next command. The module will reboot automatically after 0.5 second of idle or unsuccessful transmission.

Exit command code

After receiving this command, the module returns to normal operation, taking the new parameters' values except the I²C address.

| Start | Address | \/\ | $\Delta C K$ | Data = 0xA1 | ACK | STOP |
|-------|------------|-----|--------------|--------------|-------|------|
| Juli | / Iddi Coo | u v | , , , , , , | Duta - On II | 11011 | 3101 |













Reboot

After receiving this command, the module reboots.

| Start | Address | W | ACK | Data = 0xA2 | ACK | STOP |
|-------|---------|-----|-----|-------------|-------------|------|
| | | 0.5 | | | 2 1 7 7 7 7 | |

Typical parameter's read sequence

To read parameter(s) form the flash memory please follow steps:

- Write 0xA0 to the module start the command mode 1.
- 2. Wait 1 ms
- 3. Write 0x00...0x07 to the module – an address of the parameter
- 4. Wait 1 ms
- 5. Read 4 bytes from the module
- 6. If needed repeat steps 3-5 for another parameter
- 7. Write 0xA1 to the module – exit command mode

Typical parameter's write sequence

To write parameter(s) to the flash memory please follow steps:

- 1. Write 0xA0 to the module – start the command mode
- 2. Wait 1 ms
- 3. Write 0x20...0x25 to the module – an address of the parameter
- 4. Wait 1 ms
- 5. Write 4 bytes to the module
- 6. Wait 1 ms
- 7 If needed repeat steps 3-6 for another parameter
- Write 0xA1 to the module exit command mode or 0xA2 reboot the module

Parameter's description

Parameters: Flow A, Flow B, Flow C, Flow D are used to calculate flow from heater's power, and fluids temperature using equation:

$$flow = A + B \frac{RAW}{2^{10}} + C \left(\frac{RAW}{2^{10}}\right)^2 + D \left(\frac{RAW}{2^{10}}\right)^3$$

Where:

A: flow A, B: flow B, C: flow C, D: flow D

RAW: Raw flow value

Parameter Flow's Range limits the maximum and minimum calibrated flow's readout from the module. It should be written as the last calibration point (or slightly higher). It prohibits the user to measure the flow outside the calibration's range.













Order Information

| Description: | Item number: | Former main reference: |
|--------------|--------------|------------------------|
| SFS01 EvaKit | 105059 | 350.0033 |

Additional Products

| Description: | Item number: | Former main reference: |
|--------------|--------------|------------------------|
| SFS01 | 105050 | 350.00312 |

Order Information

| | Document name: |
|-------------------|----------------|
| Application Note: | AFSFS01_E |
| | |

